


### Chromatogram and Results

#### Injection Details

<b>Injection Name:</b> BIZ2020-D30-SCH1	<b>Injection Volume:</b> 1.00
<b>Vial Number:</b> RE5	<b>Channel:</b> UV_VIS_1
<b>Injection Type:</b> Unknown	<b>Wavelength:</b> 214
<b>Calibration Level:</b>	<b>Users:</b> jlw
<b>Instrument Method:</b> 10-90A,214NM	<b>Dilution Factor:</b> 1.0000
<b>Processing Method:</b> New Processing Method	<b>Sample Weight:</b> 1.0000
<b>Injection Date/Time:</b> 04/Jan/21 18:07	<b>Run Time (min):</b> 16.00
<b>Comment:</b> 20201230 A-RP-538	

chrom://hy261/Themo/Instrument Data/202101/20210104.seq/724.smp/UV\_VIS\_1.channel/UV\_VIS\_1.chm

#### Chromatogram

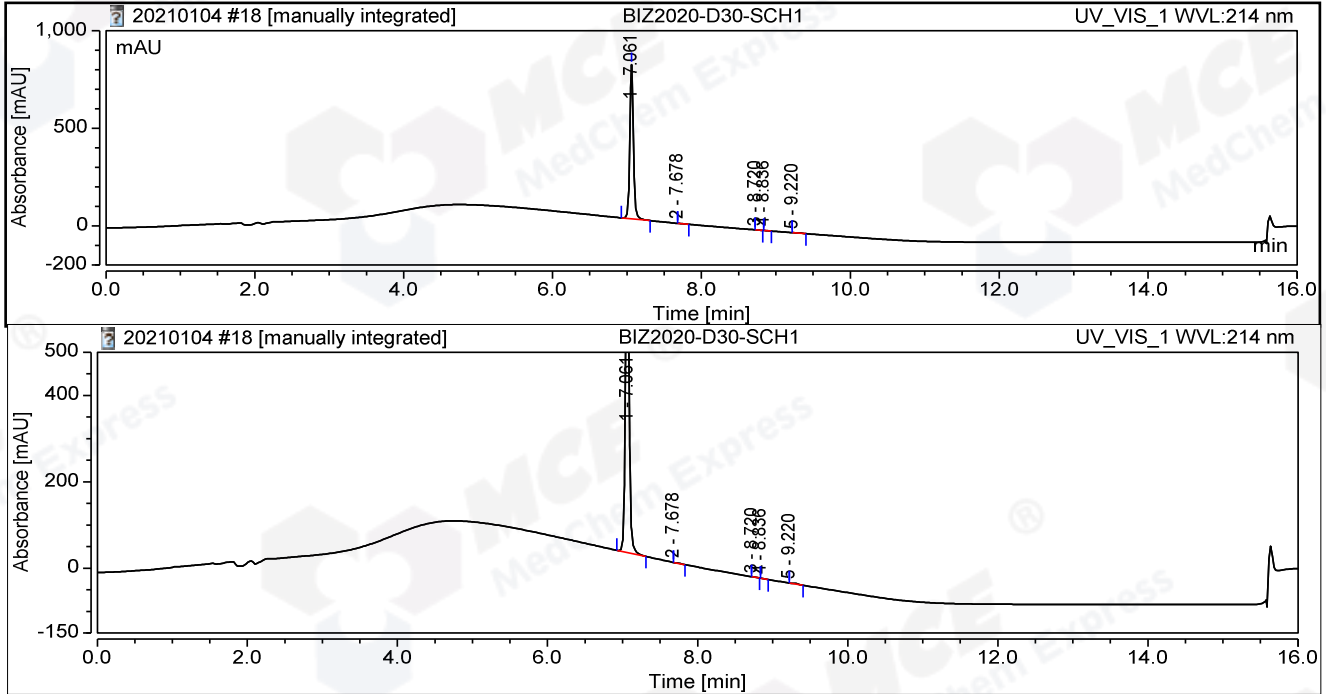

#### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Resolution (EP)	Rel.Area %
1		7.061	43.797	789.255	1.09	n.a.	99.53
2		7.678	0.051	0.000	n.a.	n.a.	0.12
3		8.720	0.017	0.000	n.a.	n.a.	0.04
4		8.836	0.016	0.000	n.a.	n.a.	0.04
5		9.220	0.122	0.000	n.a.	n.a.	0.28
<b>Total:</b>			<b>44.003</b>	<b>789.255</b>	<b>1.09</b>	<b>0.00</b>	