



File ..\DATA\2020\20201209\1193\BIZ2020-D09-SCH1.D Tgt Mass (CHM):
 Injection Date : 9 Dec 20 11:48 pm +0800 Seq. Line : 160
 Sample Name : BIZ2020-D09-SCH1 Location : P1-C-04
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20201209\1193\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20201209\1193\1-POS-3MIN.M
 CAS NO. : 2055597-12-9
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

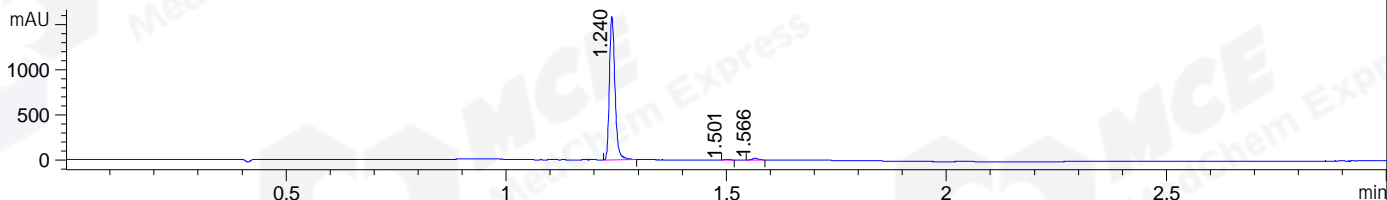


DAD1 C, Sig=254,4 Ref=off

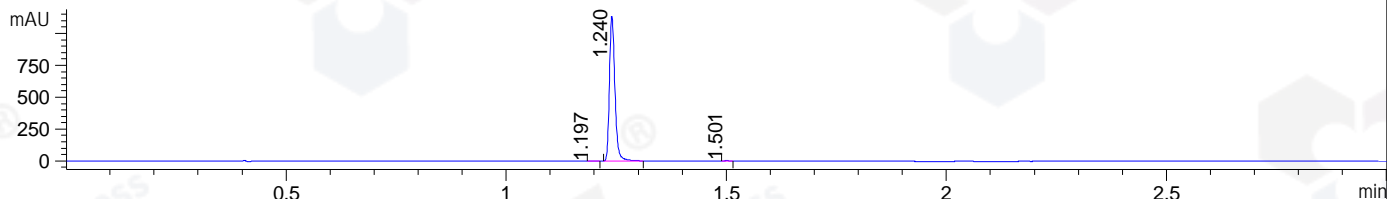

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

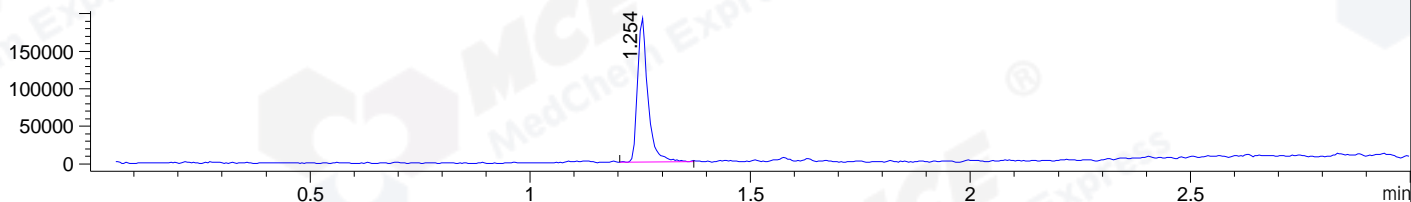

Ion 474, MSD1 474, Target Mass 473 +H Positive, EIC=473.7:474.7

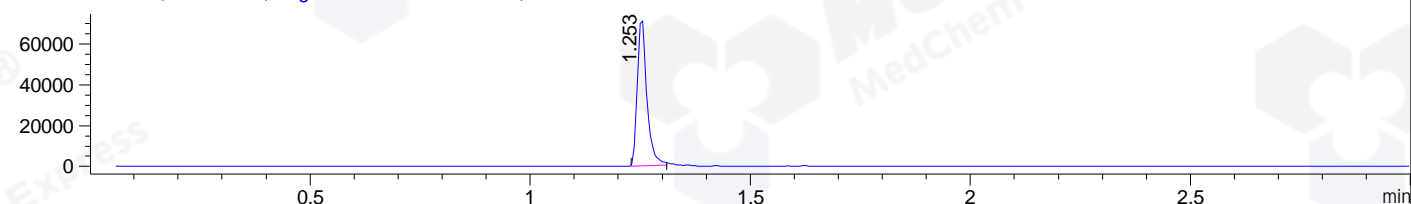

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.01	1384.87	1591.73	98.44	474
1.50	0.01	3.89	4.75	0.28	ND
1.57	0.02	18.04	18.51	1.28	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.20	0.01	1.29	1.63	0.13	ND
1.24	0.01	977.59	1138.72	99.63	474
1.50	0.01	2.35	3.06	0.24	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.02	316882.66	192689.17	100.00	474

Ret. Time: 1.25

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

