



File ..\DATA\2020\20201022\1133\BIZ2020-O19-SCH7.D Tgt Mass (CHM):  
 Injection Date : 22 Oct 20 3:08 pm +0800 Seq. Line : 7  
 Sample Name : BIZ2020-O19-SCH7 Location : P1-D-08  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20201022\1133\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20201022\1133\1-POS-3MIN.M  
 Catalog No : HY-136773A  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

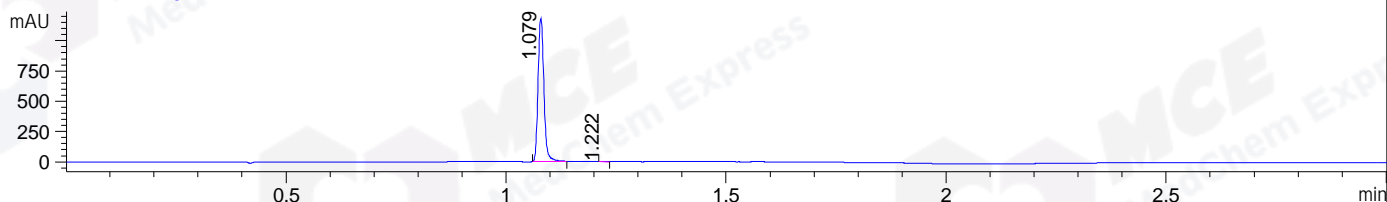


DAD1 C, Sig=254,4 Ref=off

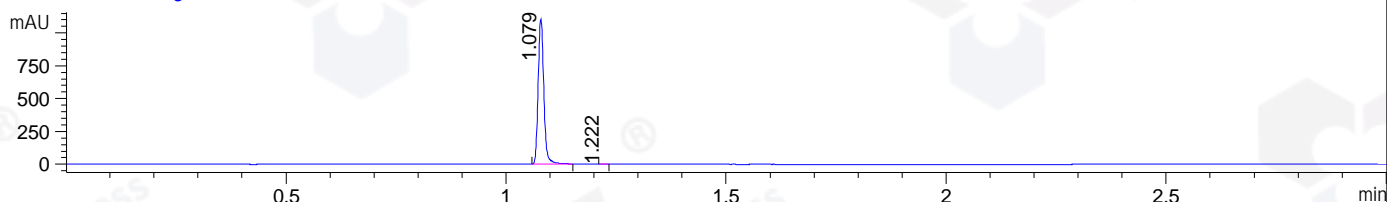

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

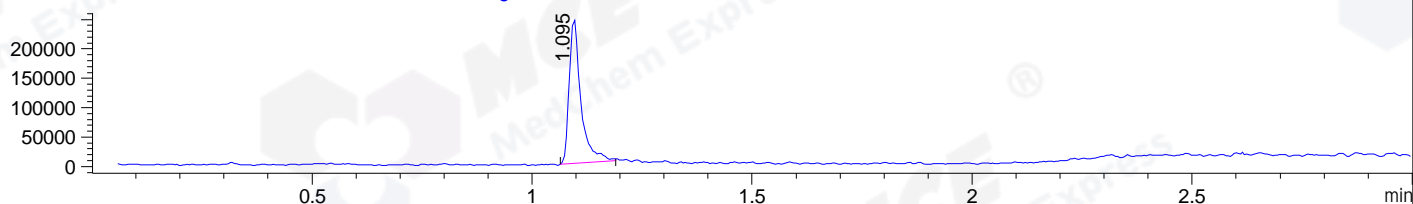

Ion 594, MSD1 594, Target Mass 593 +H Positive, EIC=593.7:594.7

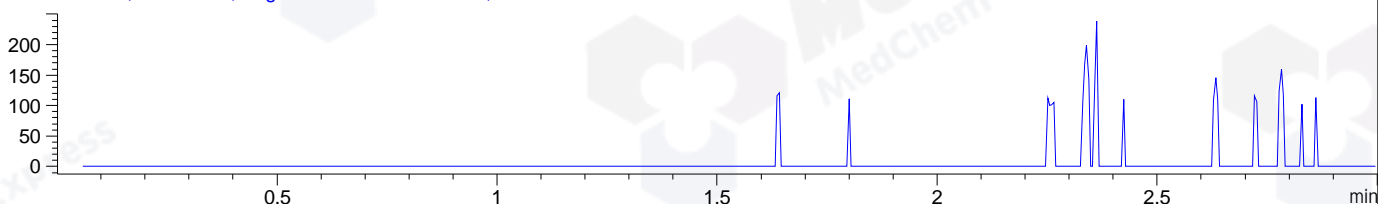

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.08	0.02	1085.24	1182.56	99.73	239
1.22	0.02	2.96	3.15	0.27	476

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.08	0.01	981.63	1105.03	99.87	239
1.22	0.01	1.26	1.71	0.13	476

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.10	0.03	456088.81	245764.39	100.00	239

Ret. Time: 1.10

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

