



File ..\DATA\2020\20200822\1080\BIZ2020-820-WLQ2.D Tgt Mass (CHM):
 Injection Date : 22 Aug 20 9:40 am +0800 Seq. Line : 9
 Sample Name : BIZ2020-820-WLQ2 Location : P1-A-07
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200822\1080\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200822\1080\1-POS-3MIN.M
 Catalog No : HY-136909
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

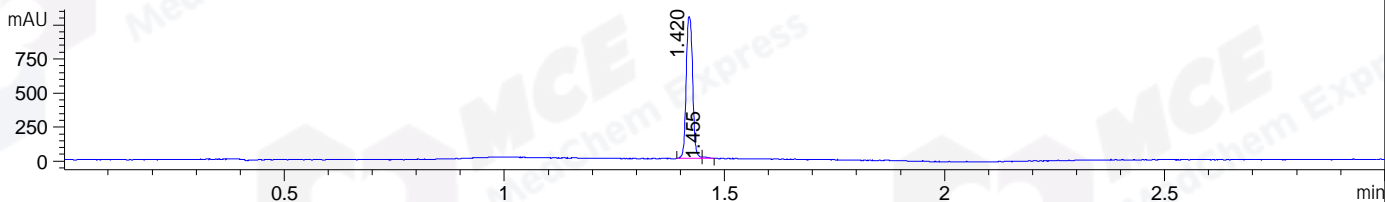


DAD1 C, Sig=254,4 Ref=off

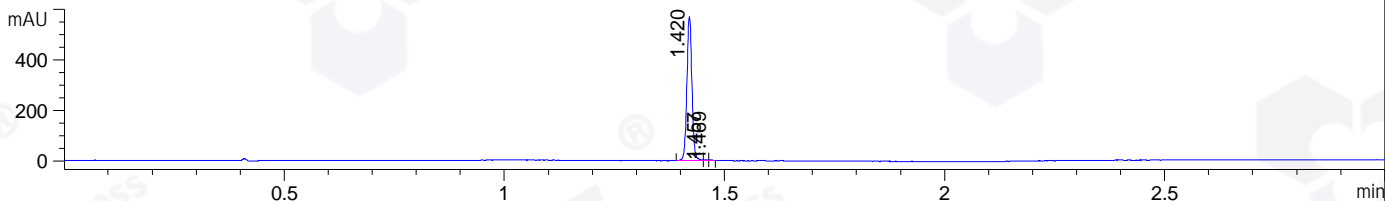

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

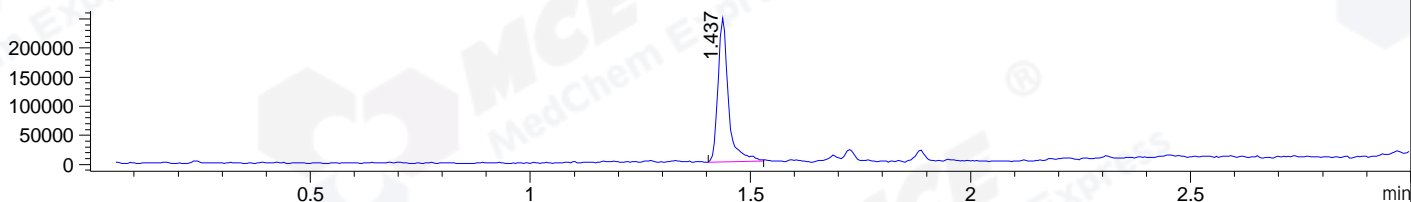

Ion 565, MSD1 565, Target Mass 564 +H Positive, EIC=564.7:565.7

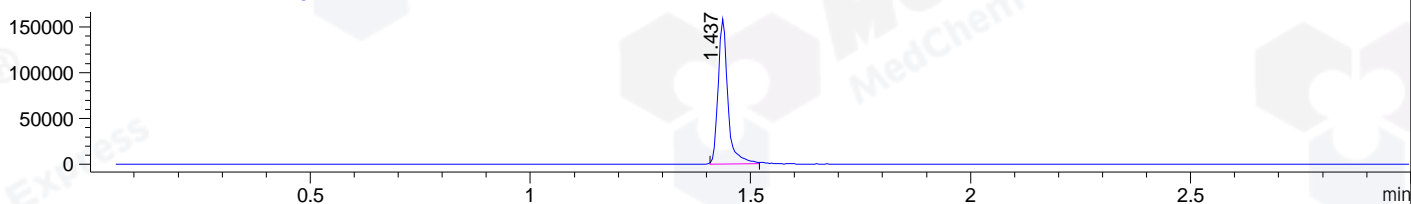

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.42	0.02	1059.62	1043.43	99.04	565
1.46	0.01	10.29	11.56	0.96	565

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.42	0.01	453.71	572.04	99.12	565
1.46	0.01	1.98	3.22	0.43	565
1.47	0.01	2.03	3.70	0.44	565

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.44	0.02	408769.00	246873.42	100.00	565

Ret. Time: 1.44

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

