



File ..\DATA\2020\20201023\1135\BIZ2020-O21-SCH8.D Tgt Mass (CHM):
 Injection Date : 23 Oct 20 8:13 pm +0800 Seq. Line : 89
 Sample Name : BIZ2020-O21-SCH8 Location : P1-D-04
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20201023\1135\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20201023\1135\1-POS-3MIN.M
 Catalog No : HY-137187
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

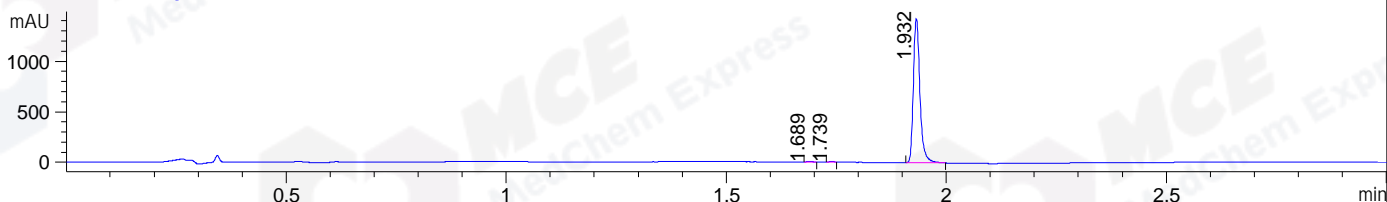


DAD1 C, Sig=254,4 Ref=off

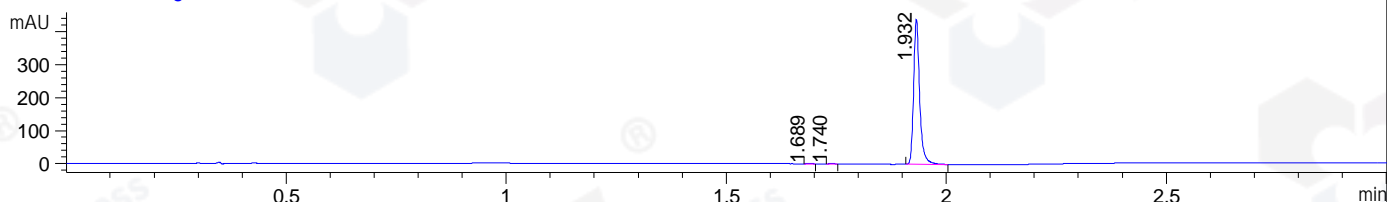

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

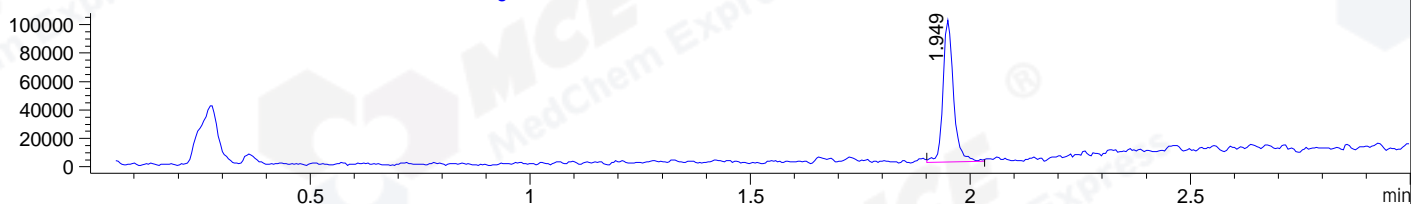

Ion 377, MSD1 377, Target Mass 376 +H Positive, EIC=376.7:377.7

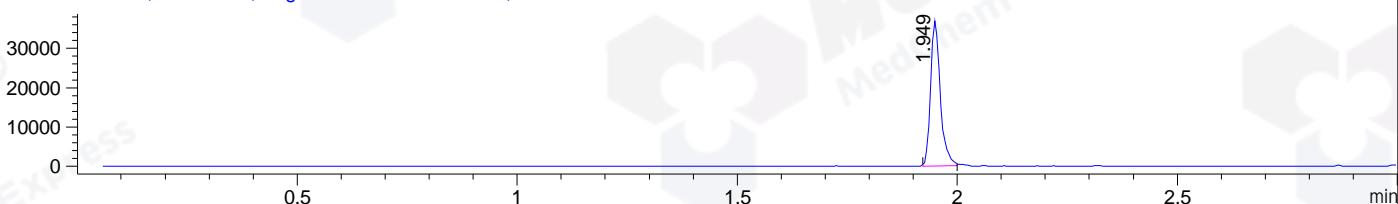

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.69	0.01	3.71	4.65	0.25	ND
1.74	0.01	3.97	5.39	0.27	279
1.93	0.02	1486.28	1427.33	99.49	377

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.69	0.01	0.67	0.90	0.16	ND
1.74	0.01	0.82	1.05	0.19	279
1.93	0.02	419.85	440.17	99.65	377

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.95	0.03	166900.89	99732.22	100.00	377

Ret. Time: 1.95

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

