



Chromatogram and Results

Injection Details

Injection Name:	WMZ9999-059-4	Run Time (min):	16.00
Vial Number:	GC7	Injection Volume:	5.00
Injection Type:	Unknown	Channel:	UV_VIS_2
Users:	jiangliwen	Wavelength:	214
Instrument Method:	HM-956_5-H01P01(RP-HPLC)	Bandwidth:	4
Processing Method:	3D Quantitative	Dilution Factor:	1.0000
Injection Date/Time:	25/Oct/2021 12:37	Sample Weight:	1
Product Name:	MRTX9768 (hydrochloride)		

chrom://hy557/DATA/Instrument Data/202110/20211025.seq/197.smp/UV_VIS_2.channel/UV_VIS_2.chm

Chromatogram

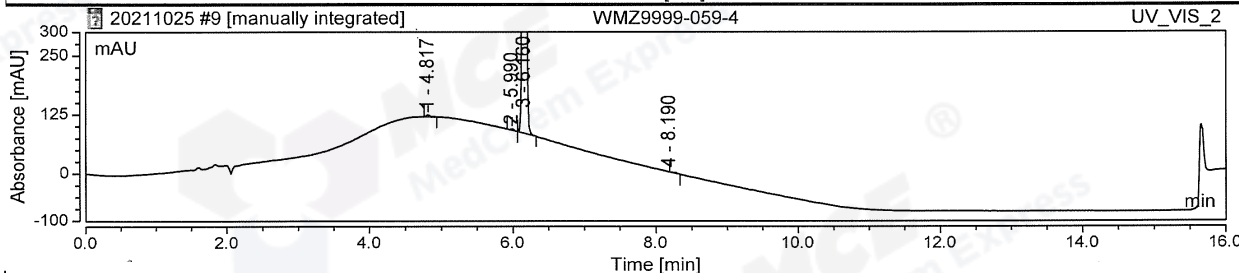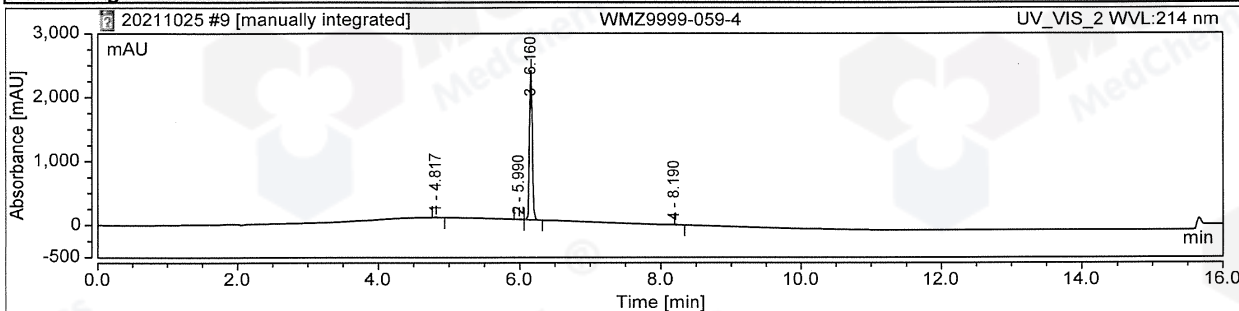

Integration Results

No.	Peak Name	Retention min	Area mAU*min	Height mAU	Resolution (EP)	Asymmetry (EP)	Rel.Area %
1		4.82	0.184	3.811	17.66	1.51	0.16
2		5.99	0.106	2.622	2.41	1.13	0.09
3		6.16	112.566	2328.431	n.a.	1.08	99.68
4		8.19	0.071	0.000	n.a.	n.a.	0.06
Total:				2334.864		20.069	3.72



Chromatogram and Results

Injection Details

Injection Name:	WMZ9999-059-4	Run Time (min):	16.00
Vial Number:	GC7	Injection Volume:	5.00
Injection Type:	Unknown	Channel:	UV_VIS_4
Users:	jiangliwen	Wavelength:	280
Instrument Method:	HM-956_5-H01P01(RP-HPLC)	Bandwidth:	4
Processing Method:	3D Quantitative	Dilution Factor:	1.0000
Injection Date/Time:	25/Oct/2021 12:37	Sample Weight:	1
Product Name:	MRTX9768 (hydrochloride)		

chrom://hy557/DATA/Instrument Data/202110/20211025.seq/197.smp/UV_VIS_4.channel/UV_VIS_4.chm

Chromatogram

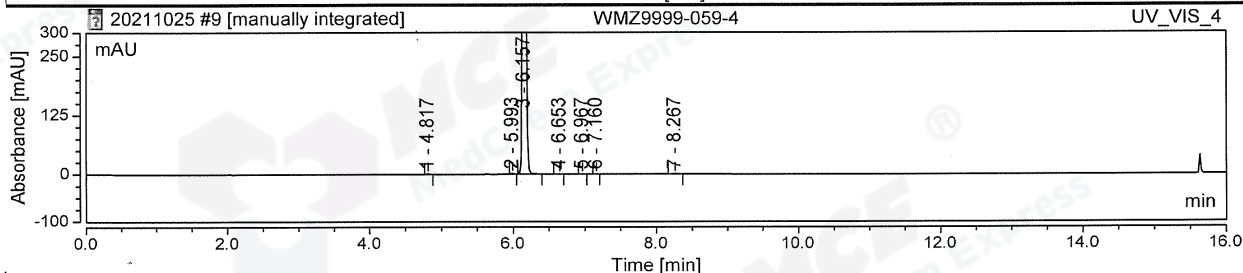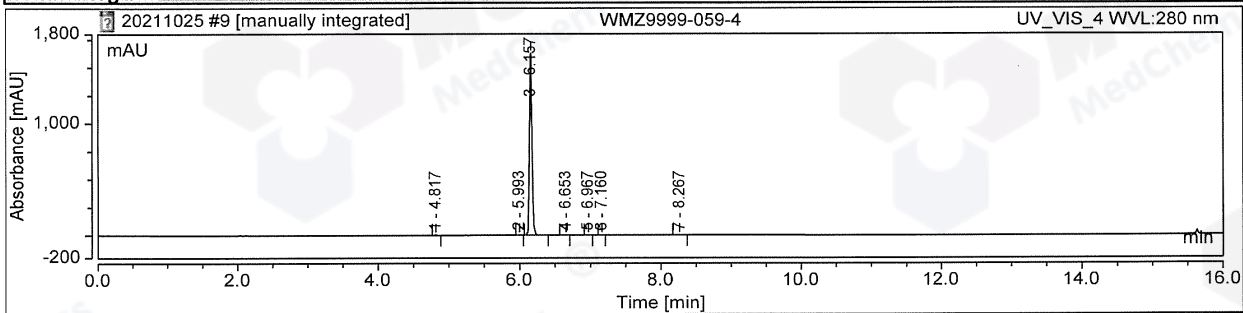

Integration Results

No.	Peak Name	Retention min	Area mAU*min	Height mAU	Resolution (EP)	Asymmetry (EP)	Rel.Area %
1		4.82	0.019	0.462	18.37	1.04	0.03
2		5.99	0.058	1.494	2.53	1.05	0.08
3		6.16	69.128	1623.909	7.25	1.17	99.76
4		6.65	0.012	0.290	4.36	1.00	0.02
5		6.97	0.012	0.252	2.60	1.08	0.02
6		7.16	0.012	0.262	14.09	0.93	0.02
7		8.27	0.051	0.973	n.a.	0.85	0.07
Total:					1627.643	49.189	7.12



Chromatogram and Results

Injection Details

Injection Name:	WMZ9999-059-4	Run Time (min):	16.00
Vial Number:	GC7	Injection Volume:	5.00
Injection Type:	Unknown	Channel:	UV_VIS_3
Users:	jiangliwen	Wavelength:	254
Instrument Method:	HM-956_5-H01P01(RP-HPLC)	Bandwidth:	4
Processing Method:	3D Quantitative	Dilution Factor:	1.0000
Injection Date/Time:	25/Oct/2021 12:37	Sample Weight:	1
Product Name:	MRTX9768 (hydrochloride)		

chrom://hy557/DATA/Instrument Data/202110/20211025.seq/1977.smp/UV_VIS_3.channel/UV_VIS_3.chm

Chromatogram

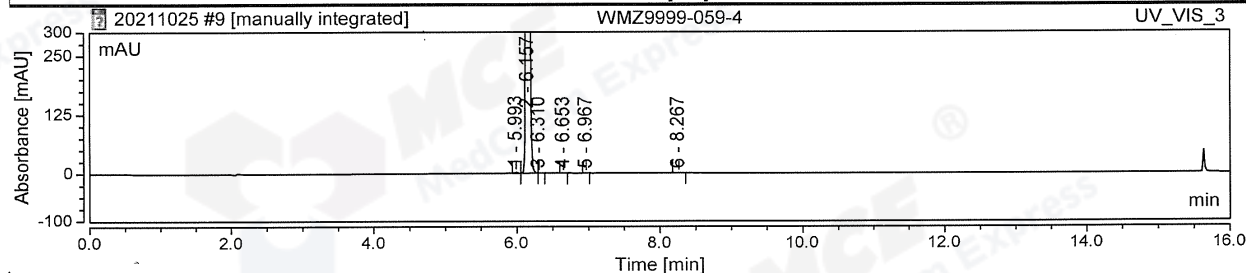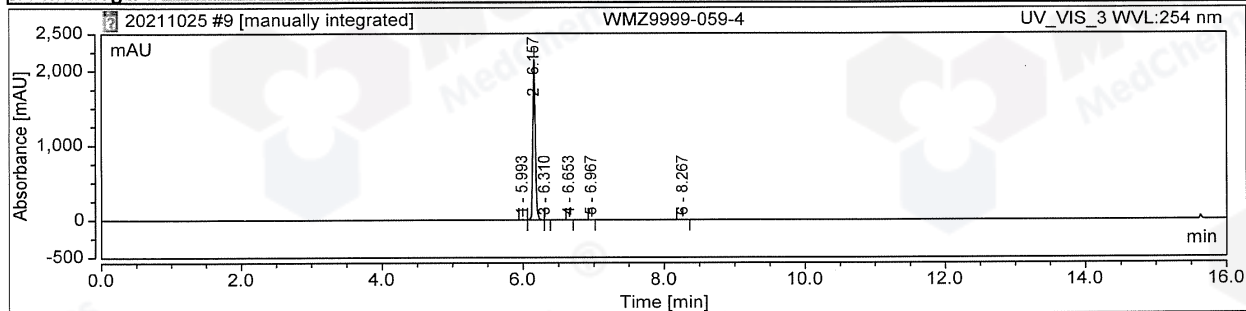

Integration Results

No.	Peak Name	Retention min	Area mAU*min	Height mAU	Resolution (EP)	Asymmetry (EP)	Rel.Area %
1		5.99	0.085	2.207	2.53	1.04	0.09
2		6.16	91.199	2146.958	n.a.	1.17	99.82
3		6.31	0.025	0.623	n.a.	n.a.	0.03
4		6.65	0.012	0.290	4.40	0.90	0.01
5		6.97	0.014	0.312	16.99	1.03	0.02
6		8.27	0.029	0.582	n.a.	0.89	0.03
Total:					2150.973	23.926	5.03