



File ..ATA\2020\20200306\861 1\CPK2020-306-11203.D Tgt Mass (CHM):
 Injection Date : 6 Mar 20 6:12 pm +0800 Seq. Line : 102
 Sample Name : CPK2020-306-11203 Location : P1-B-02
 Acq. Operator : LQ_1052 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200306\861 1\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200306\861 1\1-POS-3MIN.M
 Catalog No : HY-13998 Batch# 11203
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45□


DAD1 C, Sig=254,4 Ref=off

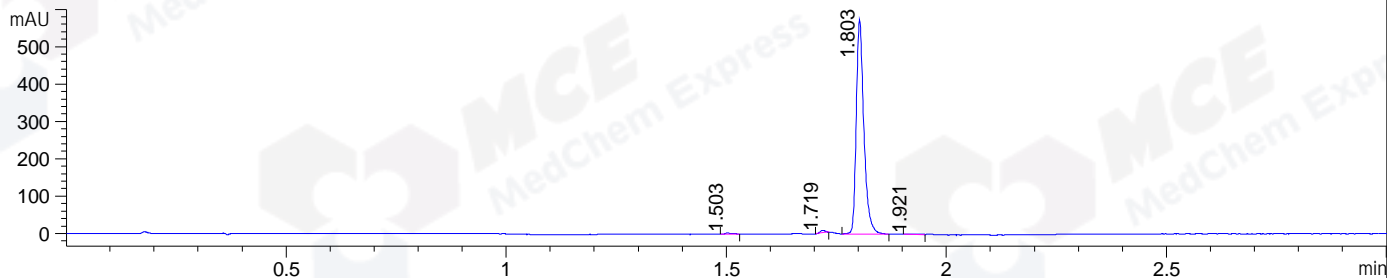

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

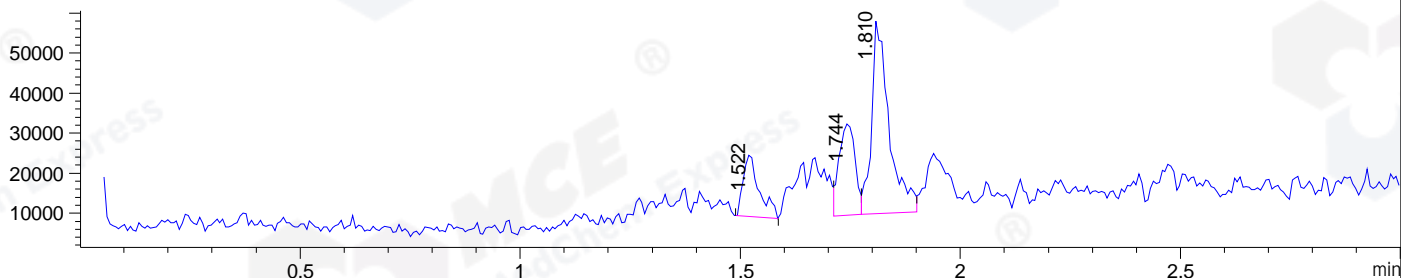

Ion 494, MSD1 494, Target Mass 493 +H Positive, EIC=493.7:494.7

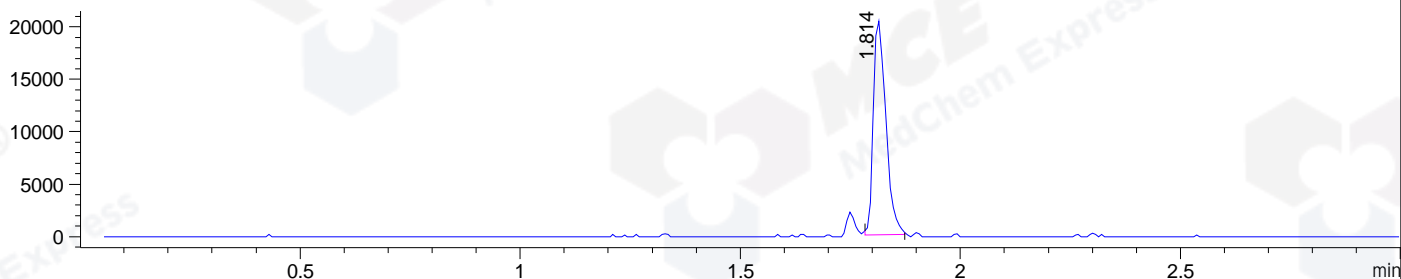


Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.50	0.02	3.89	3.44	0.56	425
1.72	0.01	4.66	6.35	0.67	279
1.80	0.02	686.09	573.23	98.40	494
1.92	0.03	2.58	1.44	0.37	250


Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.52	0.04	39006.70	15515.48	17.03	425
1.74	0.04	57448.11	22808.51	25.07	279
1.81	0.04	132652.95	49133.42	57.90	494

Ret. Time: 1.52 <<<< POSITIVE SPECTRA >>>>

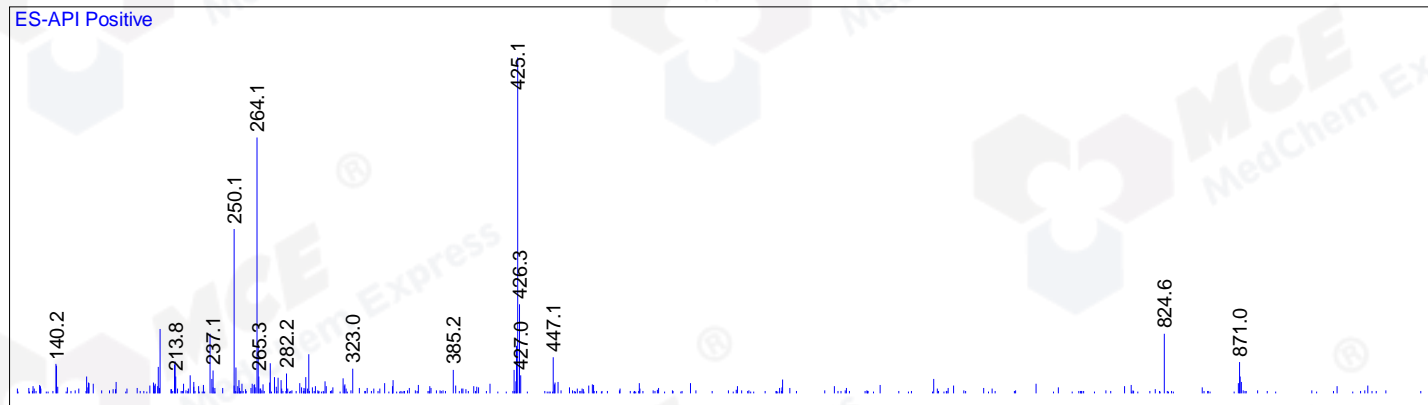

Ret. Time: 1.74

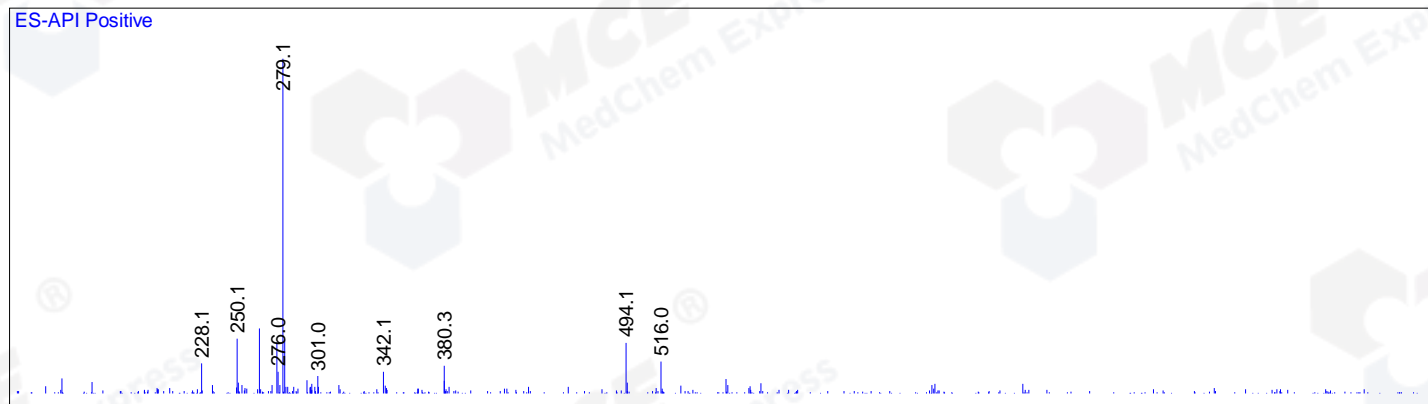

Ret. Time: 1.81

