



File ..\DATA\2019\20190416\562\BIZ2019-415-WYQ21.D Tgt Mass (CHM):  
 Injection Date : 16 Apr 19 11:44 am +0800 Seq. Line : 34  
 Sample Name : BIZ2019-415-WYQ21 Location : P1-E-04  
 Acq. Operator : LQ\_1052 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2019\20190416\562\1-POS-3MIN-1.M  
 Analysis Method : D:\CHEM32\1\DATA\2019\20190416\562\1-POS-3MIN-1.M  
 Catalog No : HY-14196 Batch#40213  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-314  
 Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

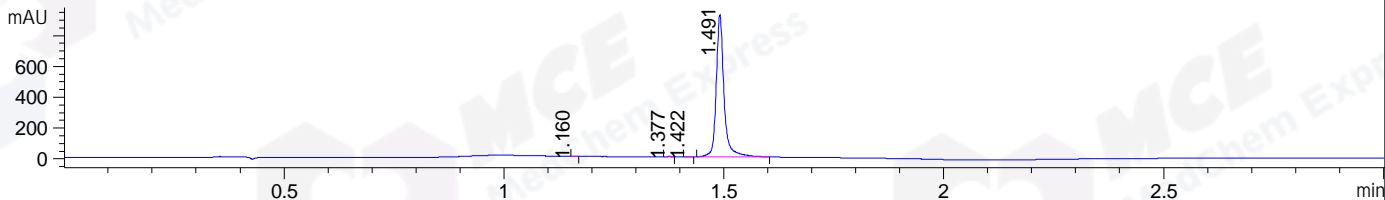


DAD1 C, Sig=254,4 Ref=off

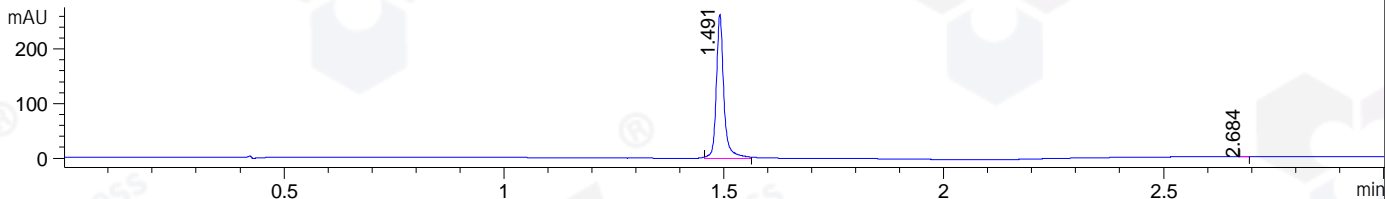

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

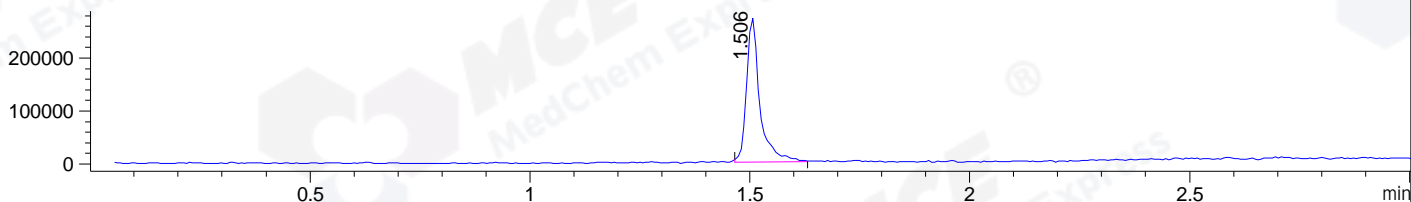

Ion 208, MSD1 208, Target Mass 207 +H Positive, EIC=207.7:208.7

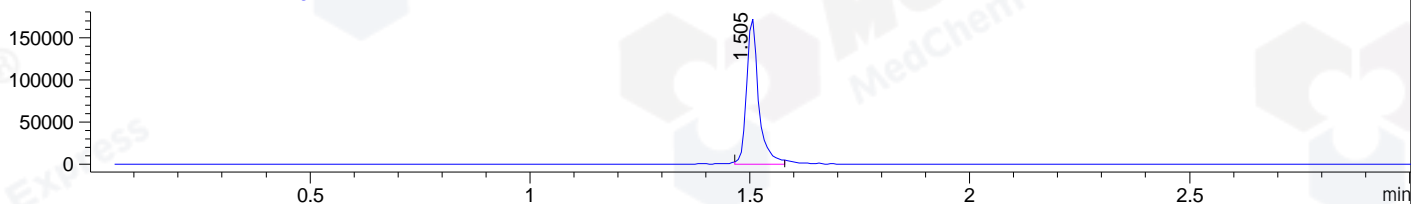

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.16	0.01	0.18	0.34	0.02	ND
1.38	0.01	1.18	1.64	0.10	ND
1.42	0.01	0.60	0.69	0.05	ND
1.49	0.02	1139.12	944.32	99.83	208

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.49	0.02	313.79	251.39	99.95	208
2.68	0.01	0.16	0.20	0.05	142

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.51	0.03	574769.63	272515.38	100.00	208

Ret. Time: 1.51

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

