



File ..\DATA\2020\20200903\1097\BIZ2020-902-WLQ6.D Tgt Mass (CHM):
 Injection Date : 3 Sep 20 7:48 pm +0800 Seq. Line : 129
 Sample Name : BIZ2020-902-WLQ6 Location : P1-C-06
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200903\1097\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200903\1097\1-POS-3MIN.M
 Catalog No : HY-14282A
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

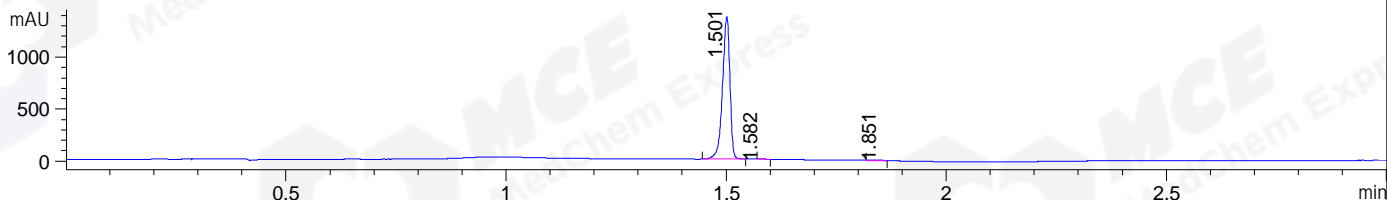


DAD1 C, Sig=254,4 Ref=off

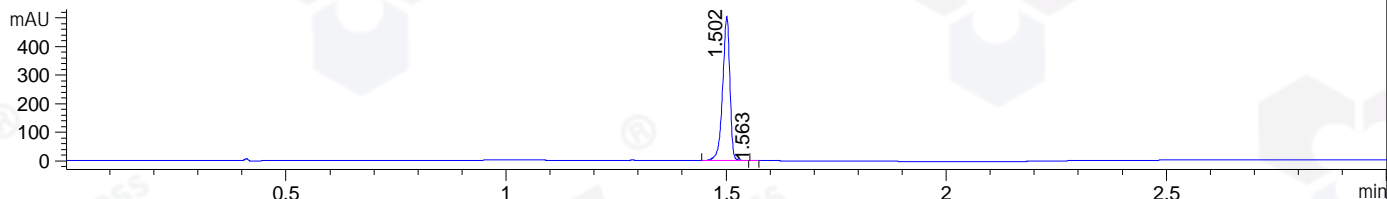

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

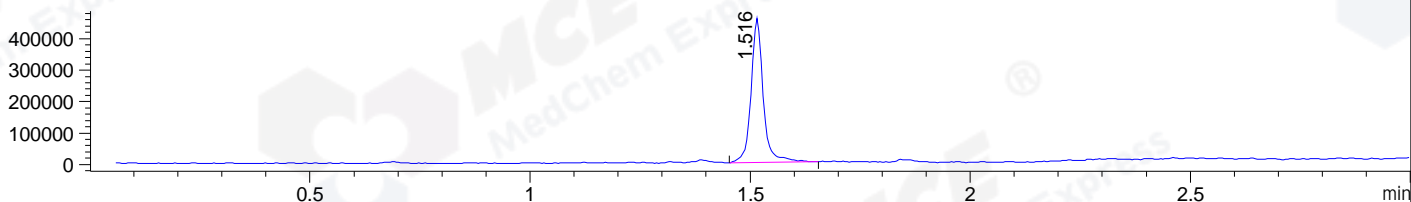

Ion 320, MSD1 320, Target Mass 319 +H Positive, EIC=319.7:320.7

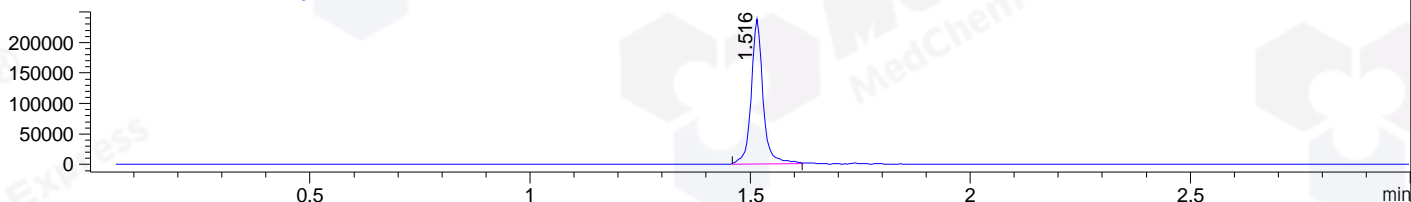

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.50	0.02	1600.21	1371.98	99.31	320
1.58	0.01	2.53	2.86	0.16	320
1.85	0.03	8.51	4.91	0.53	295

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.50	0.02	573.27	504.49	99.93	320
1.56	0.01	0.41	0.56	0.07	320

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.52	0.03	880730.50	458626.53	100.00	320

Ret. Time: 1.52

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

