



File ..DATA\2020\20201030\1141\BIZ2020-027-WLQ11.D Tgt Mass (CHM):
Injection Date : 30 Oct 20 1:42 pm +0800 Seq. Line : 62
Sample Name : BIZ2020-027-WLQ11 Location : P1-B-01
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20201030\1141\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20201030\1141\1-POS-3MIN.M
Catalog No : HY-14340
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

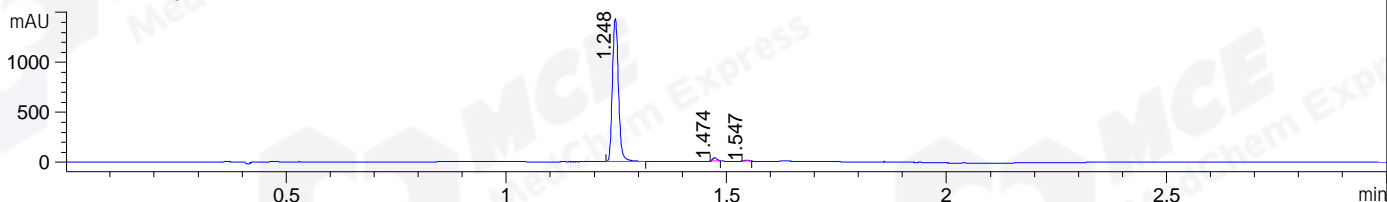


DAD1 C, Sig=254,4 Ref=off

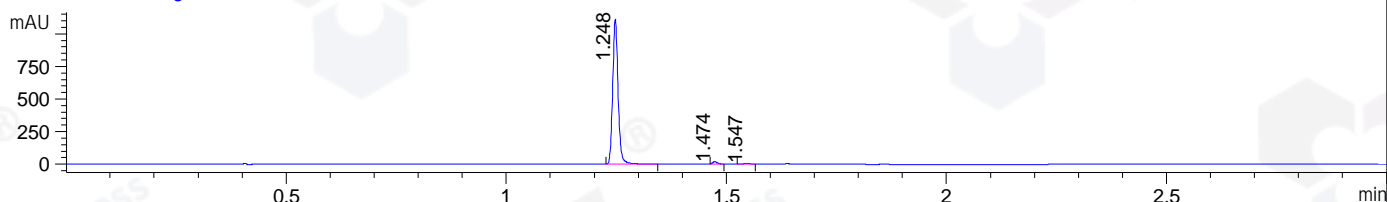

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

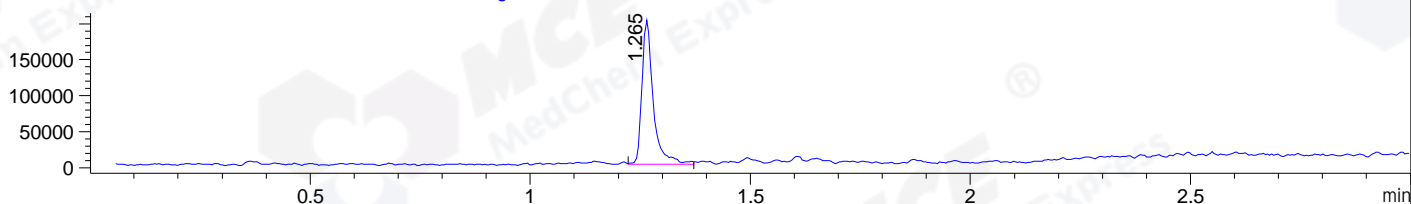

Ion 381, MSD1 381, Target Mass 380 +H Positive, EIC=380.7:381.7

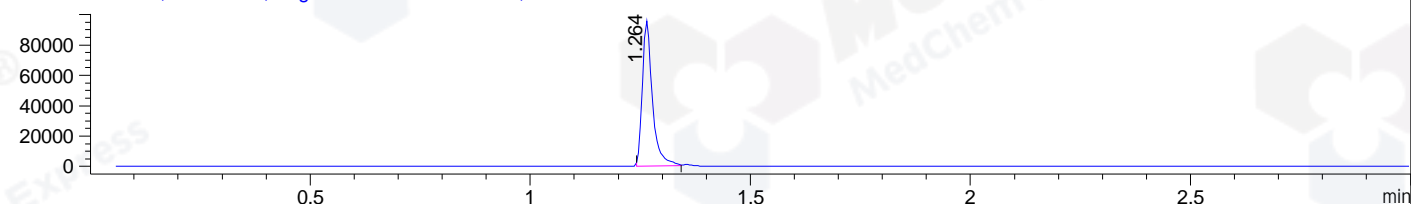

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.02	1369.36	1432.98	98.05	381
1.47	0.01	21.76	31.75	1.56	130
1.55	0.01	5.55	8.38	0.40	130

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.01	947.54	1113.46	98.05	381
1.47	0.01	13.54	17.64	1.40	130
1.55	0.02	5.28	5.82	0.55	130

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.26	0.03	361308.34	200513.45	100.00	381

Ret. Time: 1.26

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

