


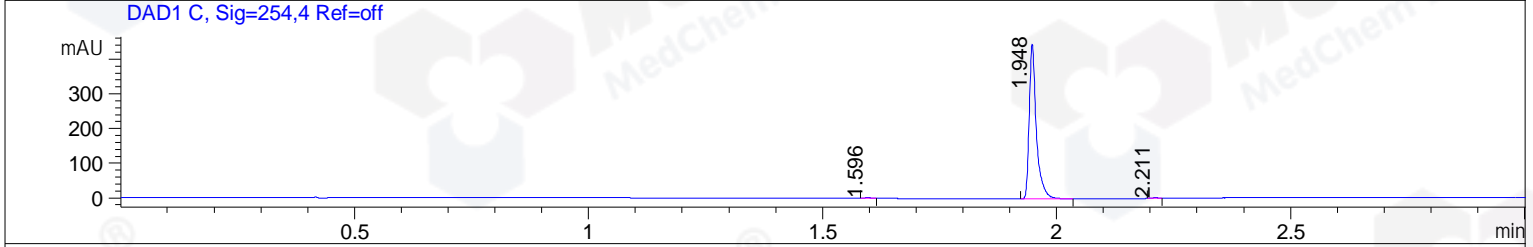


File ..DATA\2020\20200531\980\CPK2020-522-25046-.D Tgt Mass (CHM):
 Injection Date : 31 May 20 5:38 pm +0800 Seq. Line : 103
 Sample Name : CPK2020-522-25046 Location : P2-A-01
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.4 ul
 Acq. Method : D:\Chem32\1\data\2020\20200531\980\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200531\980\1-POS-3MIN.M
 Catalog No : HY-14393
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45



Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.48	0.01	1.02	1.17	0.15	214
1.60	0.01	1.47	2.15	0.21	ND
1.95	0.02	692.85	652.83	99.39	271
2.21	0.01	1.78	2.09	0.26	261

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.60	0.02	1.69	1.81	0.35	ND
1.95	0.02	475.62	447.05	99.33	271
2.21	0.01	1.49	1.68	0.31	261

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.96	0.03	35068.03	20640.31	100.00	271

Ret. Time: 1.96

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

