


=====  
Acq. Operator : Wang Ke Cheng(LCMS-02) Seq. Line : 59  
Acq. Instrument : HY-LCMS-02 Location : P1-B-02  
Injection Date : 2/2/2016 2:04:07 PM Inj : 1  
Inj Volume : 3.000 µl  
Acq. Method : D:\AGLIENT 1260\DATA\20160202\20160202 2016-02-02 09-02-49\100-1000MS+3MIN-1.5\_(0.02%FA).M  
Last changed : 2/2/2016 9:02:49 AM by Wang Ke Cheng(LCMS-02)  
Analysis Method : D:\AGLIENT 1260\DATA\20160202\20160202 2016-02-02 09-02-49\100-1000MS+3MIN-1.5\_(0.02%FA).M (Sequence Method)  
Last changed : 2/2/2016 2:17:46 PM by Wang Ke Cheng(LCMS-02)  
(modified after loading)  
Method Info : Postive,MS:100-1000,Column ID:A-RP-132,40°C  
Catalog No : HY-14423 Batch#19416  
A-RP-134

Additional Info : Peak(s) manually integrated

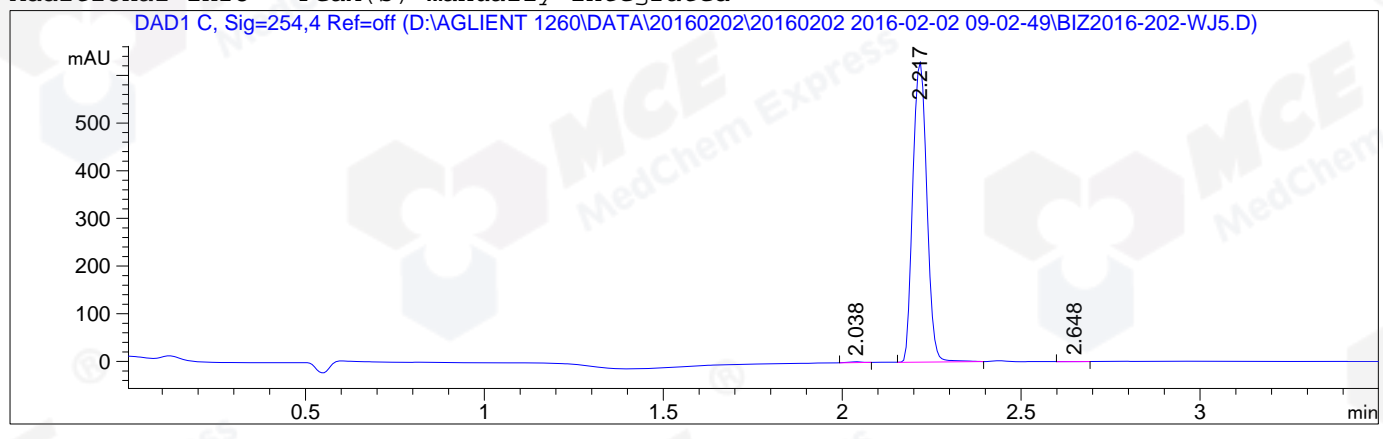

=====  
Area Percent Report  
=====

Sorted By : Signal  
Multiplier : 1.0000  
Dilution : 1.0000  
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 C, Sig=254,4 Ref=off


Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.038	MM	0.0432	4.64148	1.79167	0.2698
2	2.217	MM	0.0450	1714.20740	634.80237	99.6507
3	2.648	BB	0.0418	1.36742	5.34465e-1	0.0795

Totals : 1720.21629 637.12850

=====  
\*\*\* End of Report \*\*\*  
=====


=====  
Acq. Operator : Wang Ke Cheng(LCMS-02) Seq. Line : 59  
Acq. Instrument : HY-LCMS-02 Location : P1-B-02  
Injection Date : 2/2/2016 2:04:07 PM Inj : 1  
Inj Volume : 3.000 µl  
Acq. Method : D:\AGLIENT 1260\DATA\20160202\20160202 2016-02-02 09-02-49\100-1000MS+3MIN-1.5\_(0.02%FA).M  
Last changed : 2/2/2016 9:02:49 AM by Wang Ke Cheng(LCMS-02)  
Analysis Method : D:\AGLIENT 1260\DATA\20160202\20160202 2016-02-02 09-02-49\100-1000MS+3MIN-1.5\_(0.02%FA).M (Sequence Method)  
Last changed : 2/2/2016 2:13:58 PM by Wang Ke Cheng(LCMS-02)  
(modified after loading)  
Method Info : Postive,MS:100-1000,Column ID:A-RP-132,40°C  
Catalog No : HY-14423 Batch#19416  
A-RP-134

Additional Info : Peak(s) manually integrated

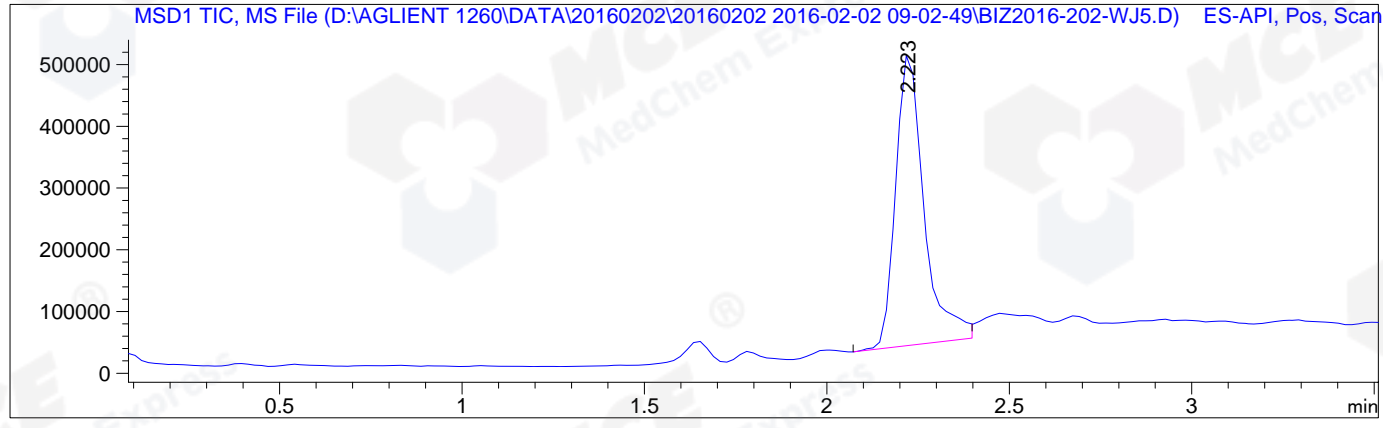

MS Signal: MSD1 TIC, MS File, ES-API, Pos, Scan, Frag: 50  
Spectra averaged over upper half of peaks.  
Noise Cutoff: 1000 counts.  
Reportable Ion Abundance: > 10%.

Retention Time (MS)	MS Area	Mol. Weight or Ion
2.223	2544000	430.20 I
		409.20 I
		408.20 I

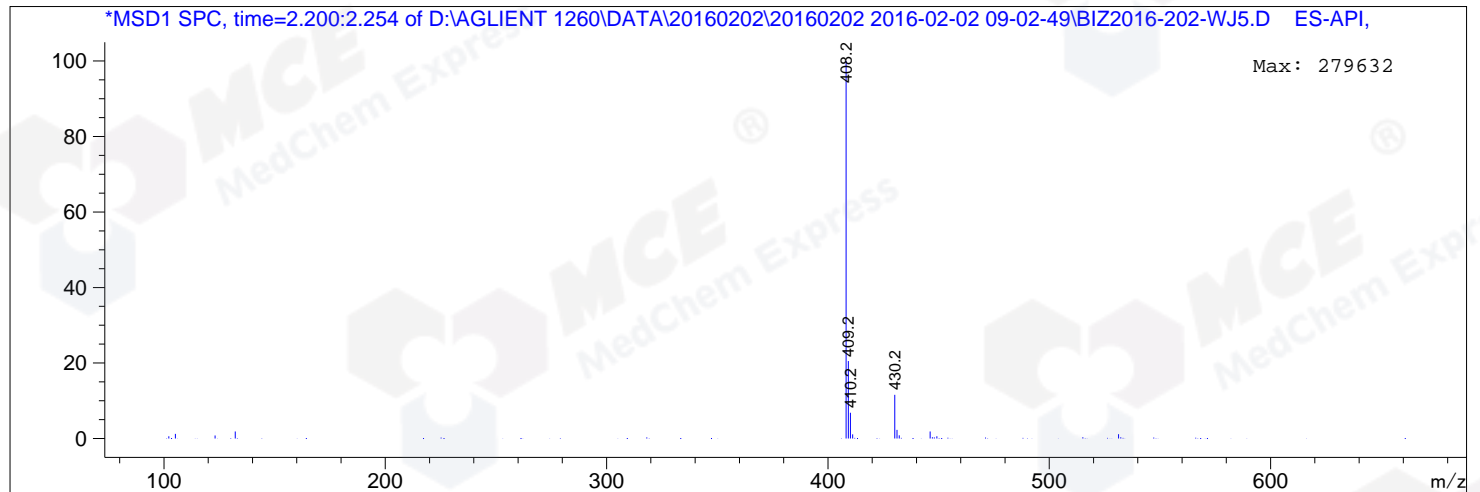

\*\*\* End of Report \*\*\*