



File ..DATA\2021\20210407\1338\CPK2021-406-32655.D Tgt Mass (CHM):
 Injection Date : 7 Apr 21 1:16 pm +0800 Seq. Line : 54
 Sample Name : CPK2021-406-32655 Location : P1-B-07
 Acq. Operator : yrz_1364 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.5 ul
 Acq. Method : D:\Chem32\1\data\2021\20210407\1338\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210407\1338\1-POS-3MIN.M
 CAS NO. : 129722-12-9
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

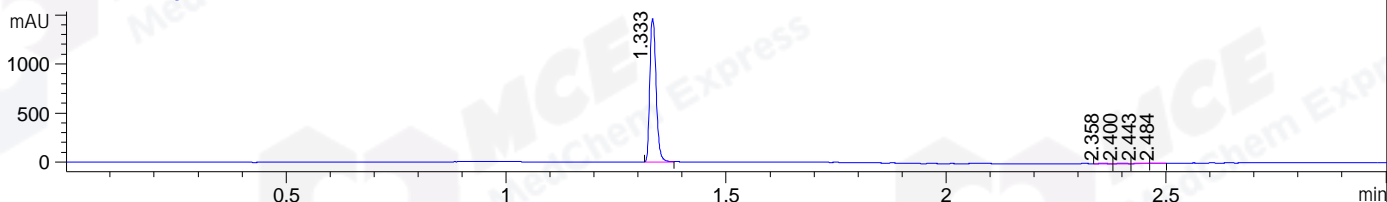


DAD1 C, Sig=254,4 Ref=off

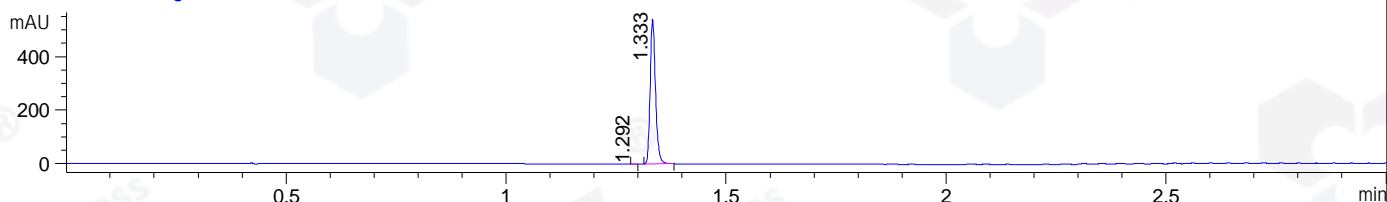

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

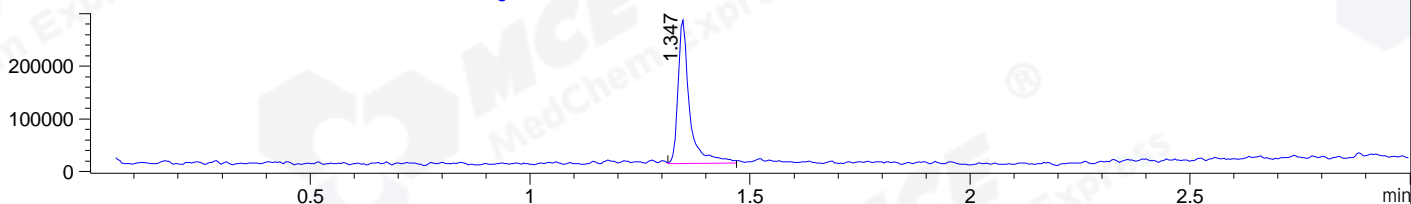

Ion 448, MSD1 448, Target Mass 447 +H Positive, EIC=447.7:448.7

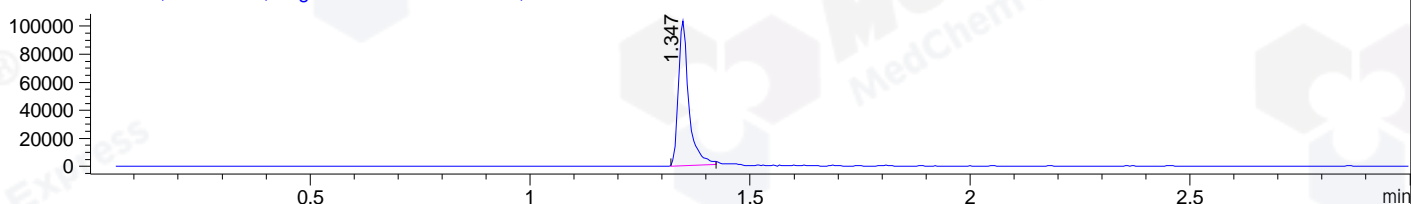

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.33	0.02	1456.98	1462.87	98.39	448
2.36	0.02	6.55	5.17	0.44	219
2.40	0.02	6.46	5.27	0.44	219
2.44	0.02	6.25	5.01	0.42	219
2.48	0.02	4.66	4.00	0.31	235

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.29	0.01	0.19	0.31	0.04	203
1.33	0.01	457.39	541.29	99.96	448

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.35	0.03	496802.66	274679.38	100.00	448

Ret. Time: 1.35

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

