



File ..\DATA\2020\20200228\854\CPK2020-227-09582.D Tgt Mass (CHM):  
 Injection Date : 28 Feb 20 11:47 am +0800 Seq. Line : 37  
 Sample Name : CPK2020-227-09582 Location : P1-B-02  
 Acq. Operator : ZJ\_1432 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200228\854\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200228\854\1-POS-3MIN.M  
 Catalog No : HY-14609 Batch#09582  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433  
 Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

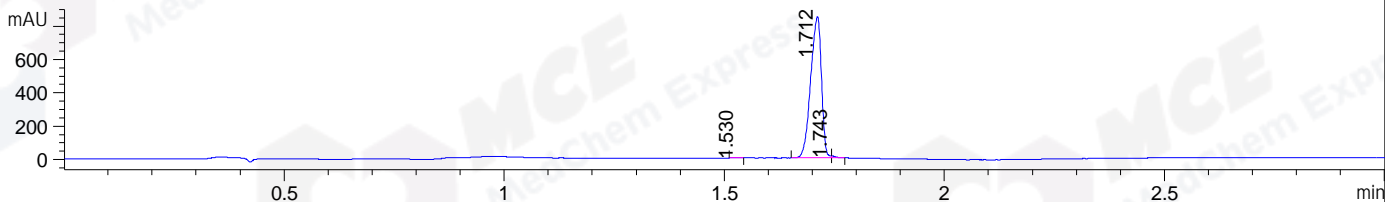


DAD1 C, Sig=254,4 Ref=off

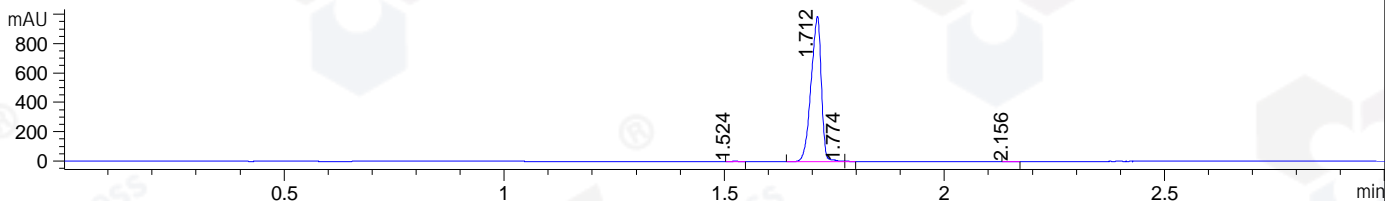

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

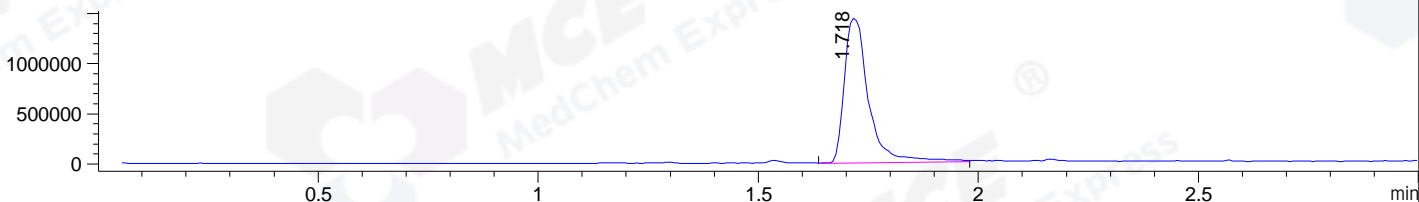

Ion 230, MSD1 230, Target Mass 229 +H Positive, EIC=229.7:230.7

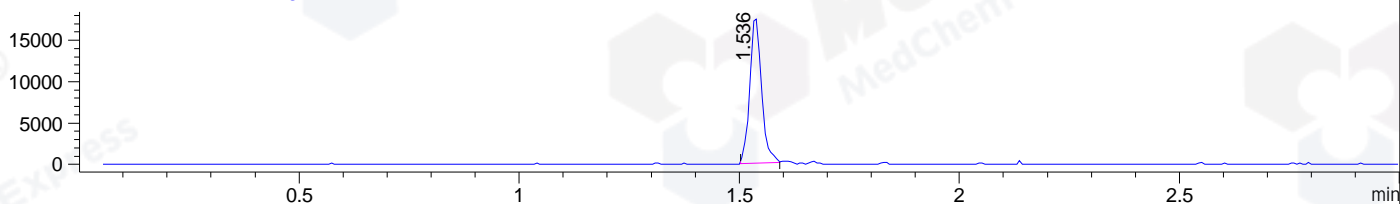

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.53	0.02	2.49	2.67	0.17	230
1.71	0.03	1442.89	848.70	99.26	194
1.74	0.01	8.33	11.99	0.57	194

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.52	0.02	1.79	1.49	0.11	230
1.71	0.03	1596.77	989.50	99.69	194
1.77	0.01	1.12	1.37	0.07	194
2.16	0.02	2.10	1.97	0.13	194

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.72	0.06	5528632.50	1443060.25	100.00	194

Ret. Time: 1.72

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

