



File ..1\DATA\2020\20200116\818\BIZ2020-115-CXL5.D Tgt Mass (CHM):
 Injection Date : 16 Jan 20 10:26 am +0800 Seq. Line : 18
 Sample Name : BIZ2020-115-CXL5 Location : P1-A-05
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200116\818\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200116\818\1-POS-3MIN.M
 Catalog No : HY-14660 Batch#59138
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

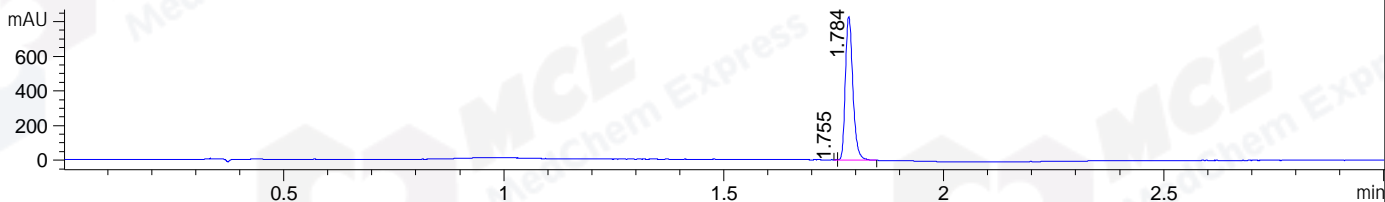


DAD1 C, Sig=254,4 Ref=off

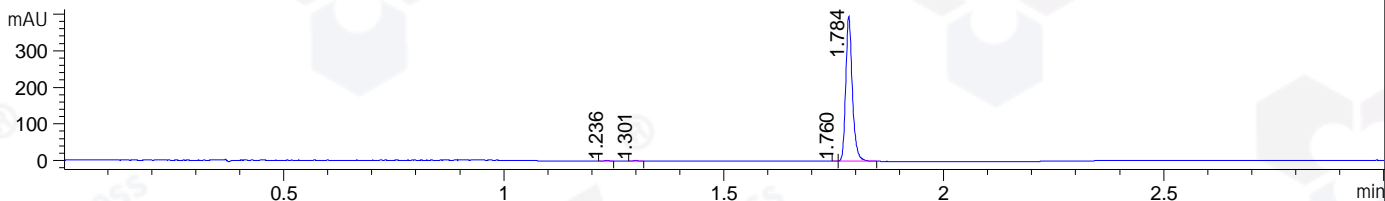

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

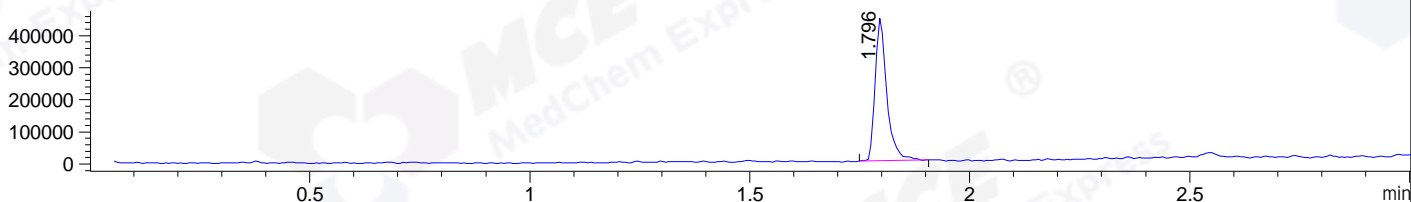

Ion 520, MSD1 520, Target Mass 519 +H Positive, EIC=519.7:520.7

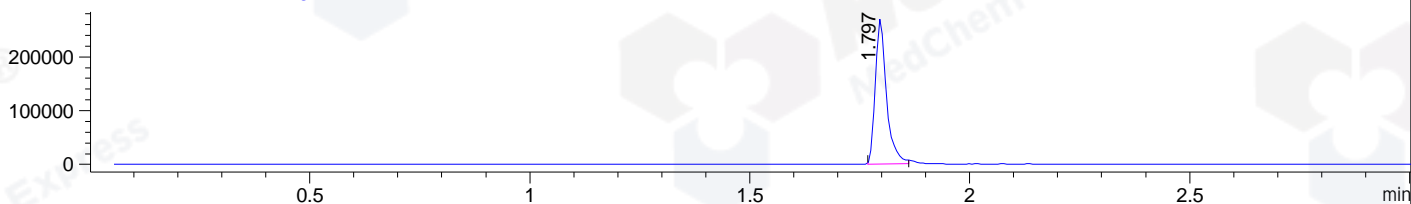

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.75	0.00	0.34	1.44	0.03	ND
1.78	0.02	983.48	828.96	99.97	520

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.01	0.63	0.86	0.15	ND
1.30	0.01	0.49	0.61	0.12	ND
1.76	0.01	0.30	0.46	0.07	ND
1.78	0.02	413.54	396.57	99.66	520

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.80	0.03	832713.25	447382.38	100.00	520

Ret. Time: 1.80

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

