
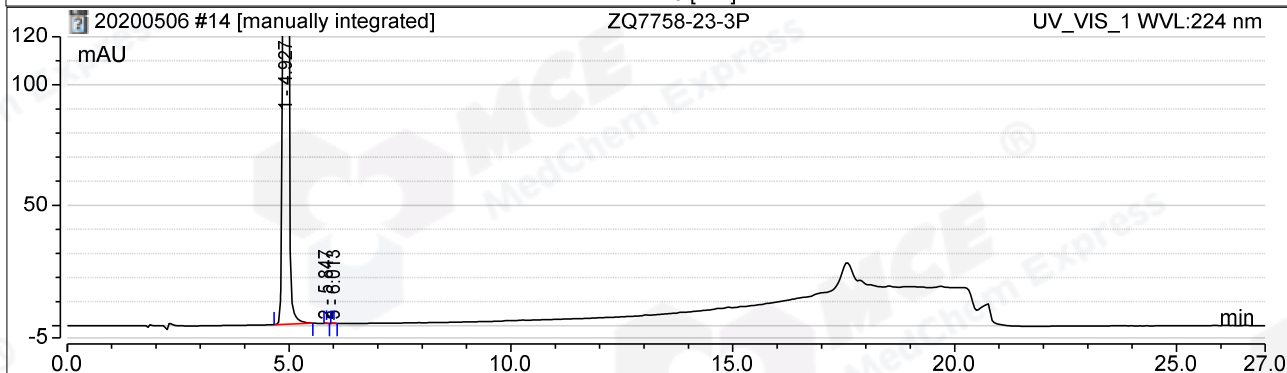


Chromatogram and Results

Injection Details

Injection Name: ZQ7758-23-3P	Run Time (min): 27.00
Vial Number: RE7	Injection Volume: 5.00
Injection Type: Unknown	Channel: UV_VIS_1
Comment: HM-153_8-20200506 A-RP-490	Wavelength: 224
Instrument Method: HM-153_8-H01P,AB,C1-6	Bandwidth: 4
Processing Method: 3D Quantitative	Dilution Factor: 1.0000
Injection Date/Time: 06/May/20 17:11	Acq Operator: gxt

Chromatogram

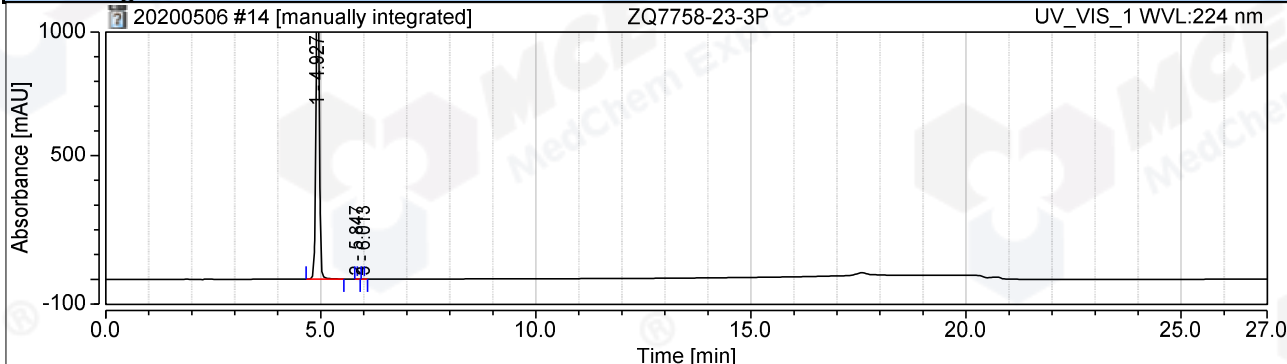

Integration Results

No.	Peak Name	Retention Time min	Area mAU*s	Height mAU	Relative Area %	Resolution	Plates	Asymmetry
1		4.927	7125.299	1433.568	99.98	7.78	23446	1.00
2		5.847	0.715	0.178	0.01	1.44	46993	1.06
3		6.013	0.599	0.125	0.01	n.a.	37390	0.95
Total:			7126.613	1433.871	100.00		107829.00	