

File ..019\20190703\20190703 1\BIZ2019-702-WYQ12.D Tgt Mass (CHM):

Injection Date : 3 Jul 19 5:31 pm +0800 Seq. Line : 71

Sample Name : BIZ2019-702-WYQ12 Location : P2-C-09

Acq. Operator : SYSTEM Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\LCMS03\Data\20190703\20190703 1\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190703\20190703 1\1-POS-3MIN.M

Catalog No : HY-14887 Batch#43076

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-446

Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

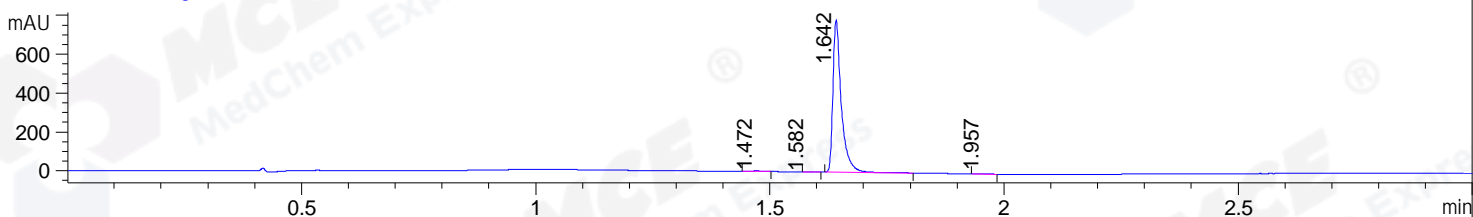


DAD1 B, Sig=254,4 Ref=off

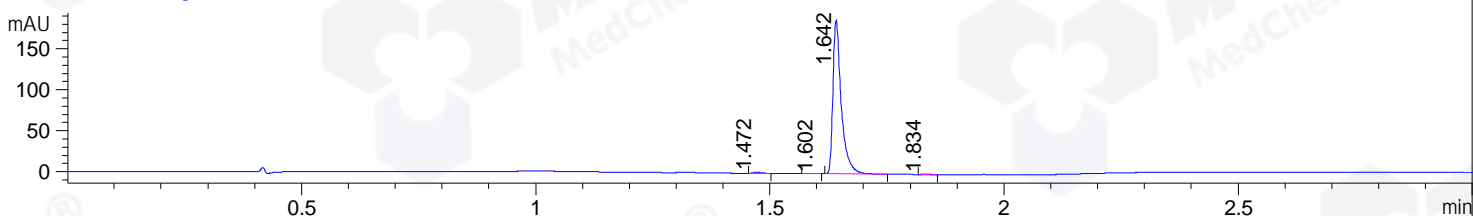

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

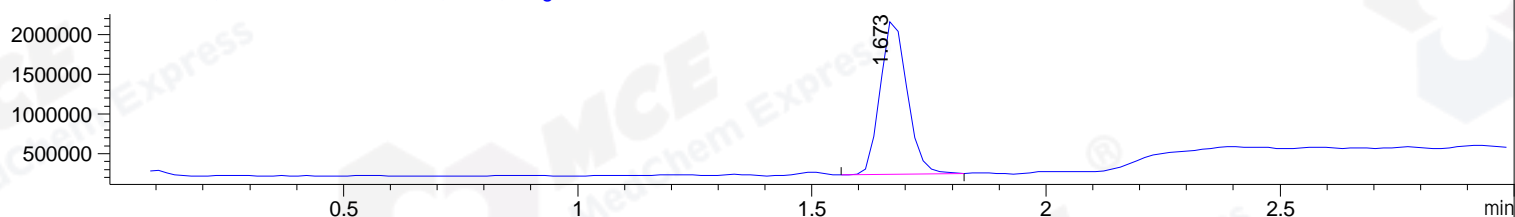

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7:1.7

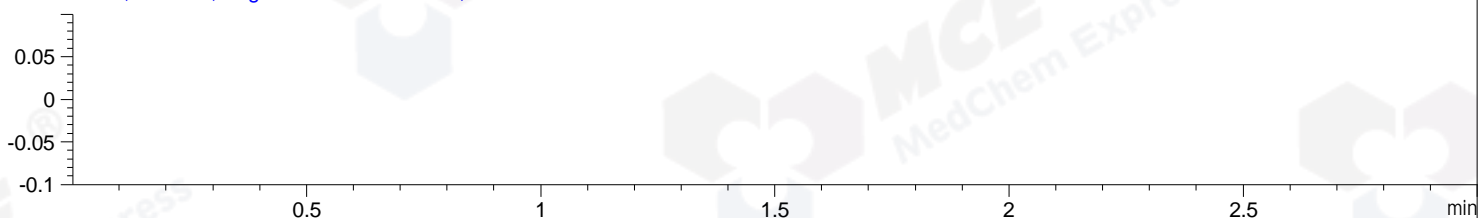

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.47	0.02	4.21	3.70	0.43	145
1.58	0.02	1.38	1.18	0.14	145
1.64	0.02	963.90	783.49	99.03	463
1.96	0.02	3.88	2.77	0.40	145

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.47	0.02	1.89	1.61	0.81	145
1.60	0.04	0.66	0.30	0.28	145
1.64	0.02	230.42	187.45	98.75	463
1.83	0.02	0.38	0.28	0.16	145

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.67	0.06	7759674.00	1966510.75	100.00	463

Ret. Time: 1.67

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

