



File ..DATA\2020\20201125\1166\CPK2020-N24-13868.D Tgt Mass (CHM):
Injection Date : 25 Nov 20 8:50 pm +0800 Seq. Line : 129
Sample Name : CPK2020-N24-13868 Location : P1-E-01
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20201125\1166\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20201125\1166\1-POS-3MIN.M
Catalog No : HY-14908
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

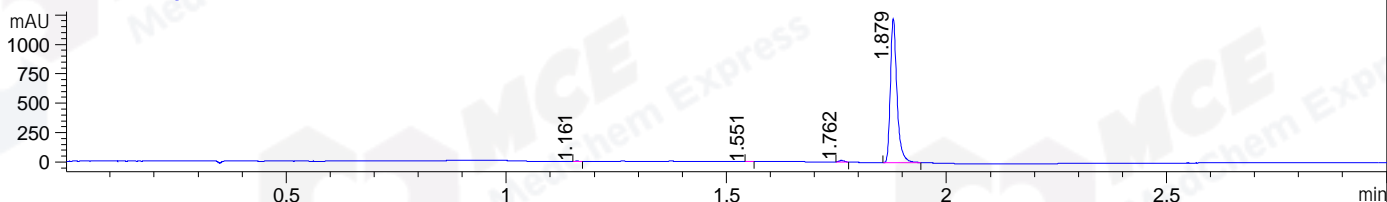


DAD1 C, Sig=254,4 Ref=off

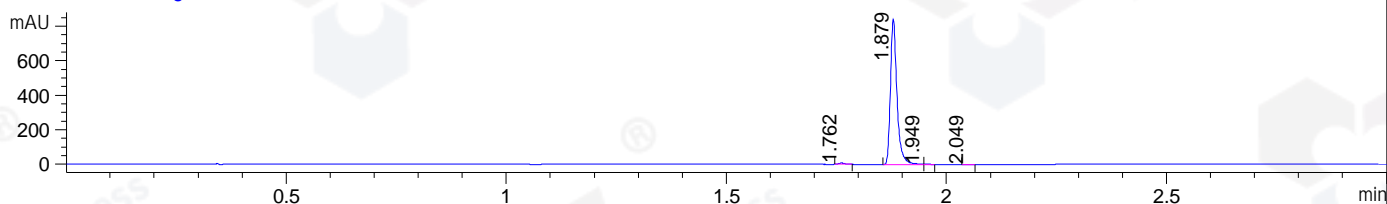

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

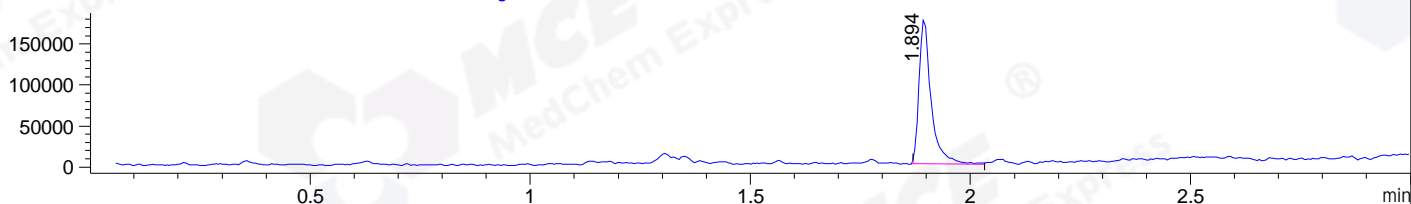

Ion 356, MSD1 356, Target Mass 355 +H Positive, EIC=355.7:356.7

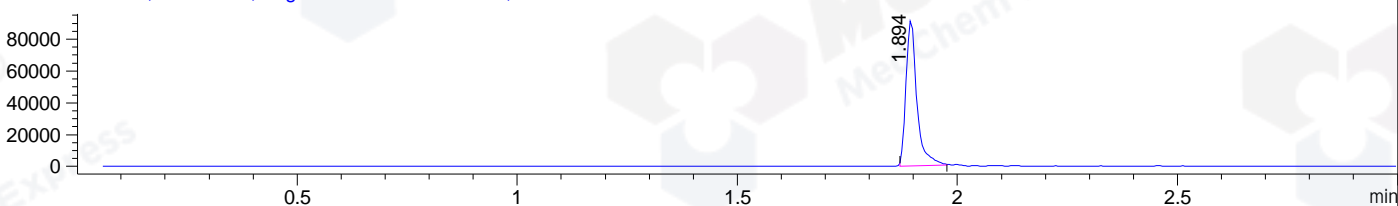

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.16	0.01	2.49	3.52	0.19	ND
1.55	0.01	1.29	2.00	0.10	ND
1.76	0.01	10.53	12.60	0.82	260
1.88	0.02	1268.07	1228.25	98.88	356

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.76	0.02	6.89	7.38	0.78	260
1.88	0.02	869.68	842.52	98.91	356
1.95	0.01	1.36	1.87	0.15	356
2.05	0.02	1.32	1.42	0.15	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.89	0.03	333085.75	175953.63	100.00	356

Ret. Time: 1.89

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

