



File ..ATA\2020\20200103\802 1\CPK2020-102-24497.D Tgt Mass (CHM):
Injection Date : 3 Jan 20 3:59 pm +0800 Seq. Line : 27
Sample Name : CPK2020-102-24497 Location : P1-B-05
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.4 ul
Acq. Method : D:\Chem32\1\data\2020\20200103\802 1\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20200103\802 1\1-POS-3MIN.M
Catalog No : HY-15084A Batch# 24497
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

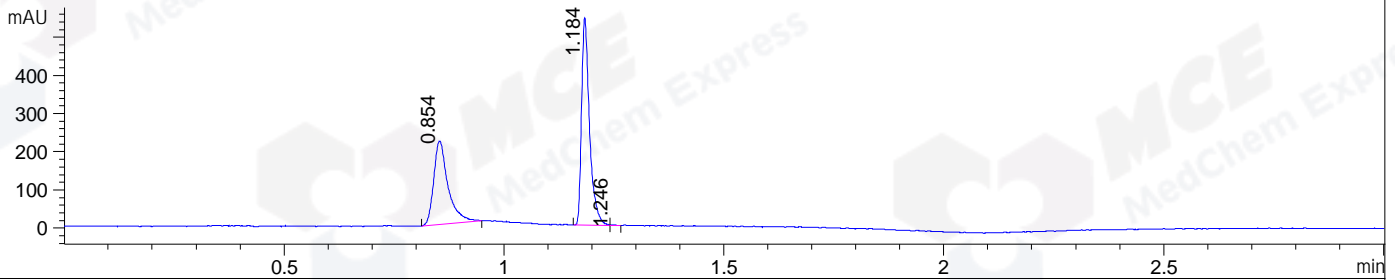

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

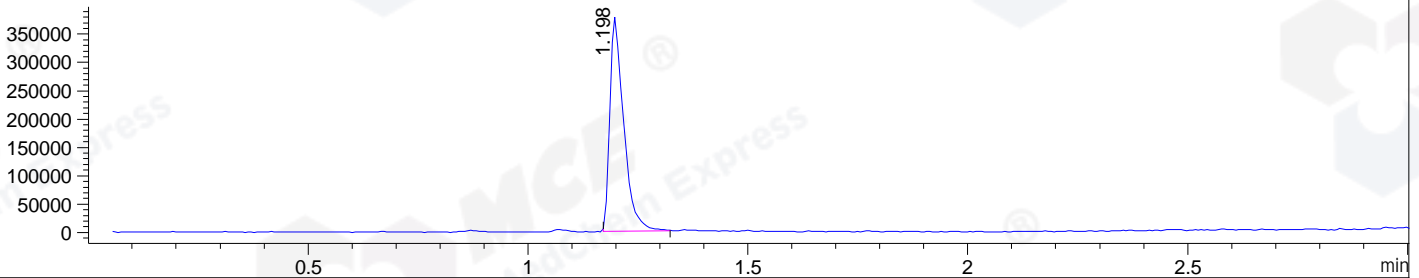

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7:1.7

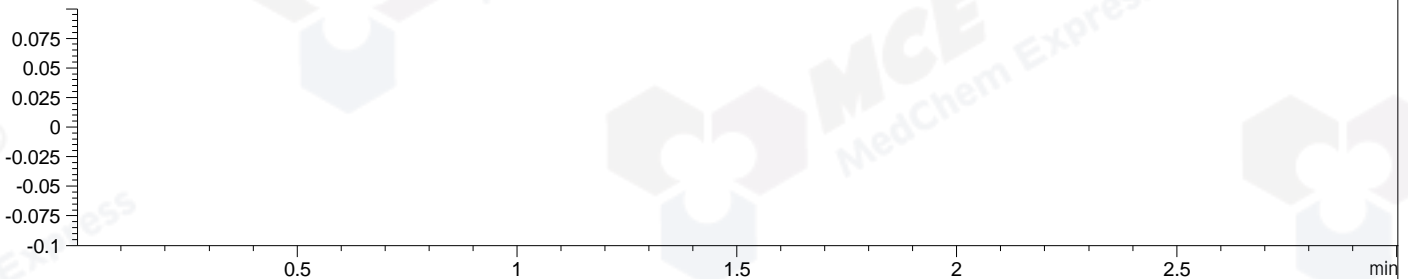

Integration Results for DAD1 B, Sig=214,4 Ref=off

| RetTim | Width | Area | Height | Area% | MS (+) |
|--------|-------|--------|--------|-------|--------|
| 0.85 | 0.04 | 498.46 | 219.24 | 42.05 | ND |
| 1.18 | 0.02 | 685.09 | 543.38 | 57.79 | 222 |
| 1.25 | 0.01 | 1.98 | 2.22 | 0.17 | 222 |

Integration Results for MSD1 TIC, MS File

| RetTim | Width | Area | Height | Area% | MS (+) |
|--------|-------|-----------|-----------|--------|--------|
| 1.20 | 0.03 | 838349.63 | 378270.69 | 100.00 | 222 |

Ret. Time: 1.20

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

