



File ..DATA\2019\20190227\543\BIZ2019-226-WYQ3.D Tgt Mass (CHM):
 Injection Date : 27 Feb 19 11:54 am +0800 Seq. Line : 28
 Sample Name : BIZ2019-226-WYQ3 Location : P1-B-01
 Acq. Operator : LQ_1052 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 2 ul
 Acq. Method : D:\Chem32\1\data\2019\20190227\543\1-POS-3MIN-1.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190227\543\1-POS-3MIN-1.M
 Catalog No : HY-15149 Batch#38348
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-314
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

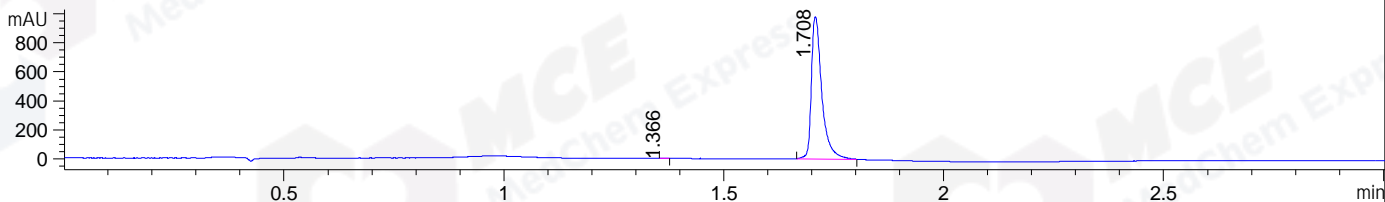


DAD1 C, Sig=254,4 Ref=off

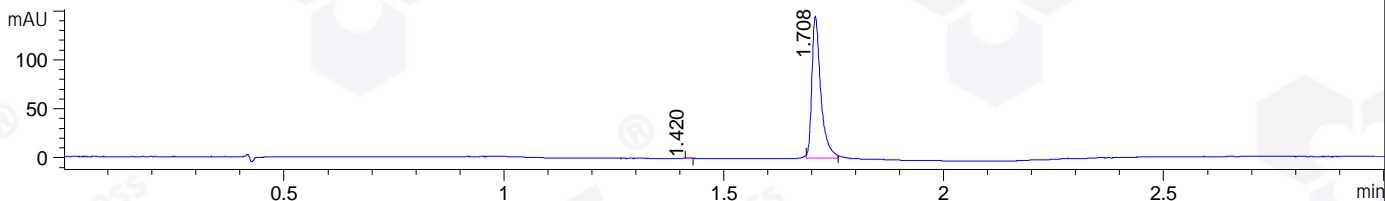

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

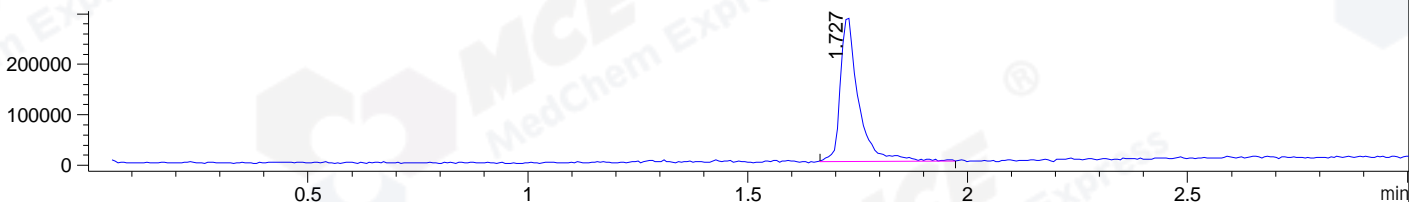

Ion 541.2, MSD1 541.2, Target Mass 540.2 +H Positive, EIC=540.9:541.9

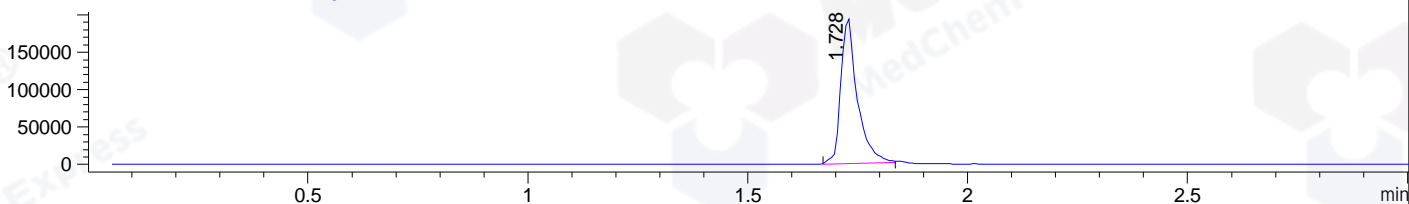

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.37	0.01	0.34	0.61	0.02	130
1.71	0.02	1642.53	986.74	99.98	541

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.42	0.01	0.12	0.23	0.06	130
1.71	0.02	204.63	145.07	99.94	541

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.73	0.04	831982.44	289203.13	100.00	541

Ret. Time: 1.73

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

