



File ..DATA\2020\20201203\1182\CPK2020-D03-16676.D Tgt Mass (CHM):  
 Injection Date : 3 Dec 20 10:11 pm +0800 Seq. Line : 131  
 Sample Name : CPK2020-D03-16676 Location : P1-B-08  
 Acq. Operator : zyj\_1547 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20201203\1182\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20201203\1182\1-POS-3MIN.M  
 CAS NO. : 1137868-52-0  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

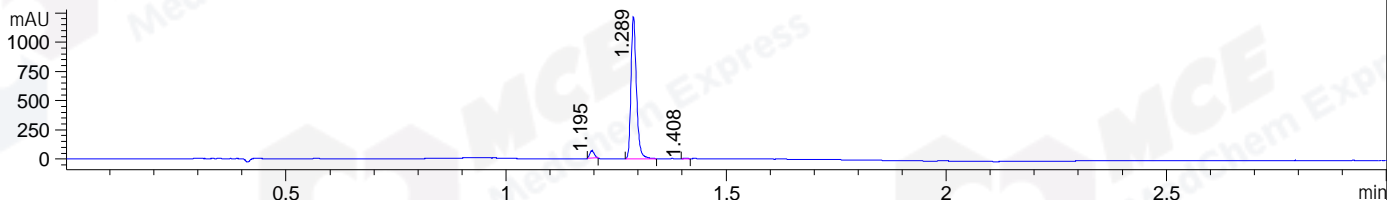


DAD1 C, Sig=254,4 Ref=off

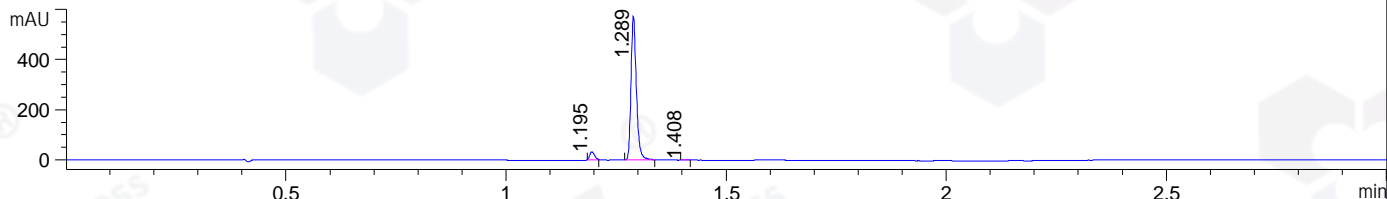

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

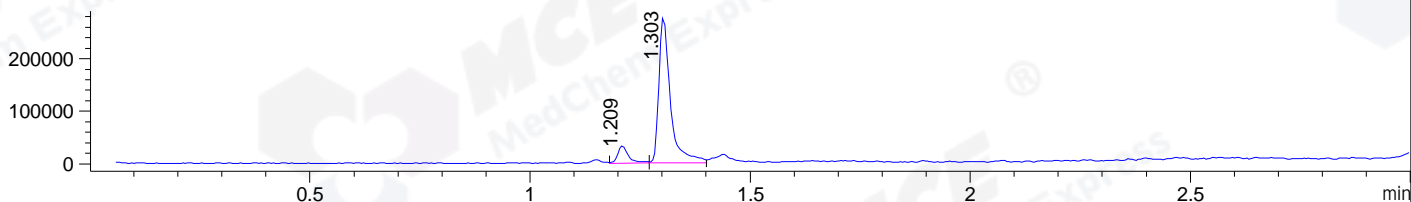

Ion 562, MSD1 562, Target Mass 561 +H Positive, EIC=561.7:562.7

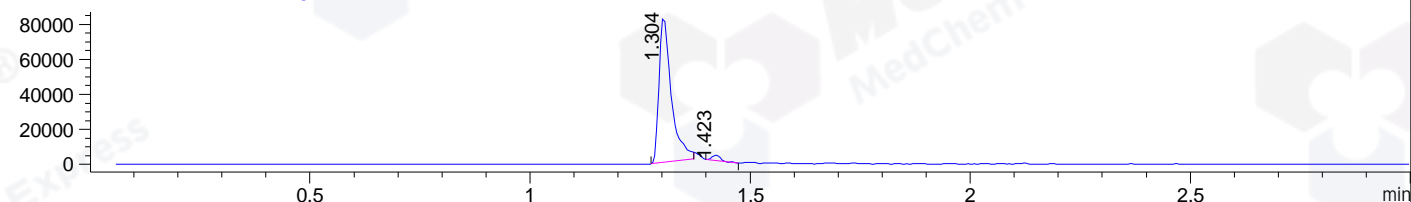

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.19	0.01	46.87	65.38	4.27	291
1.29	0.01	1047.57	1219.97	95.44	282
1.41	0.01	3.15	4.74	0.29	562

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.19	0.01	23.66	31.66	4.63	291
1.29	0.01	485.66	573.59	95.12	282
1.41	0.01	1.29	1.96	0.25	562


Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.21	0.03	55818.09	32715.89	9.91	291
1.30	0.03	507604.16	277664.78	90.09	282

Ret. Time: 1.21

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

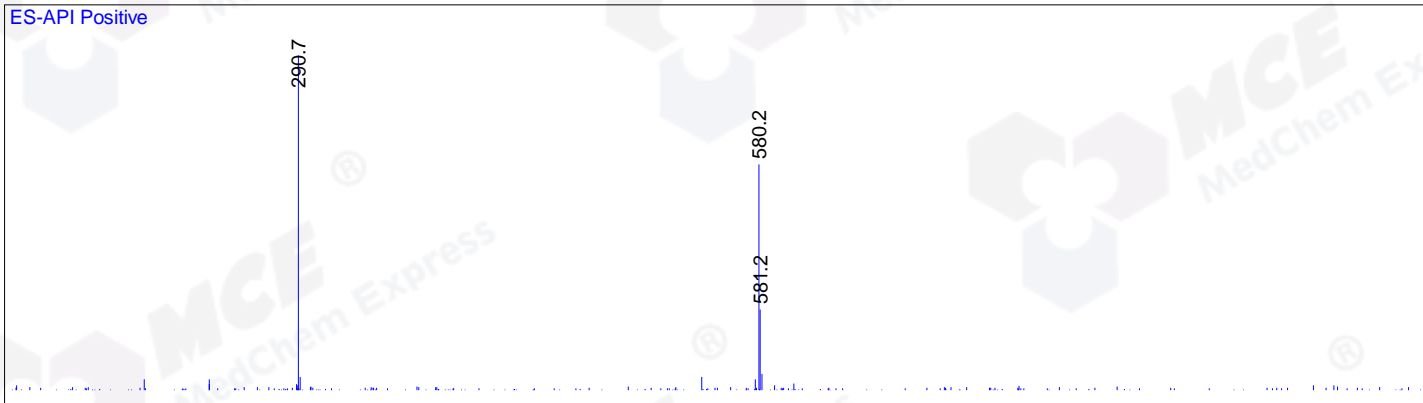

Ret. Time: 1.30

ES-API Positive

