


Sample ID:HP5434-060-2_2, Catalog No: HY-15229 Batch#32279 ,D2O

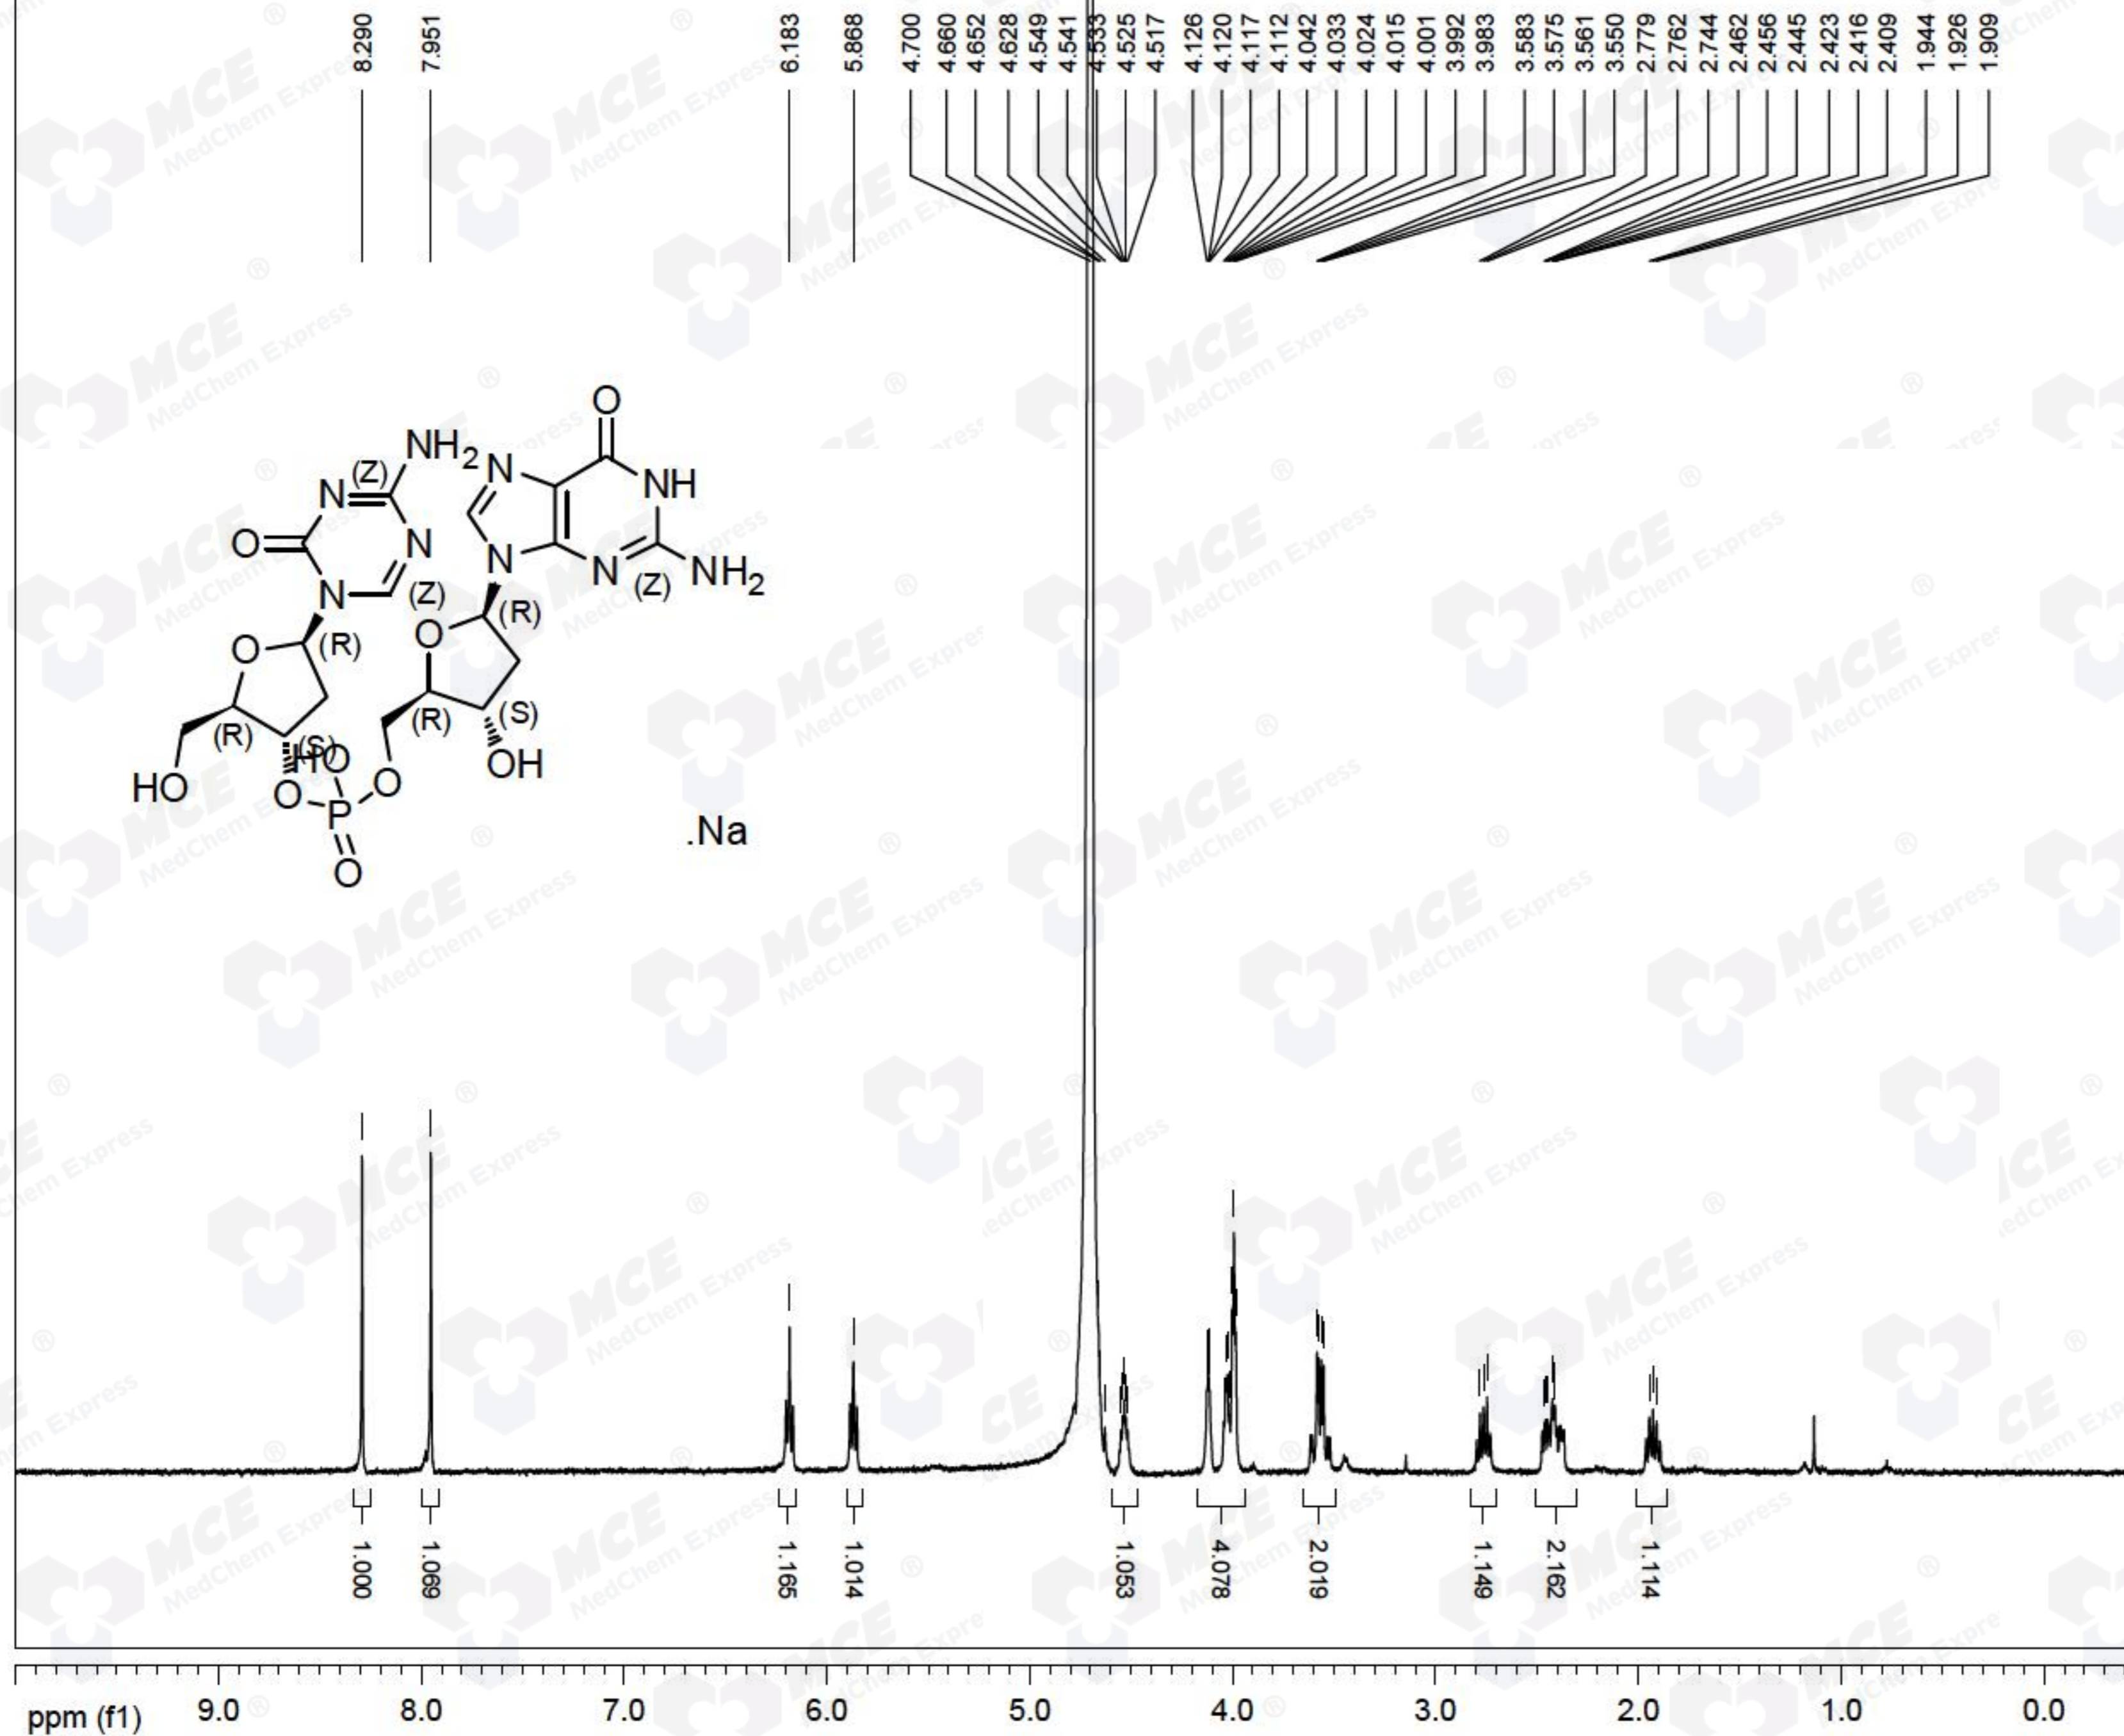

Date:

23 Aug 2018

Document's Title:

Catalog No: HY-15229 Batch#32279

Spectrum Title:

hp5434-060-2_2-d2o-180823

Frequency (MHz):

(f1) 400.132

Original Points Count:

(f1) 24670

Actual Points Count:

(f1) 65536

Acquisition Time (sec):

(f1) 2.4670

Spectral Width (ppm):

(f1) 24.992

Pulse Program:

ZG30

Temperature:

297.76

Number of Scans:

16

Acq. Date:

Thu Aug 23 11:46:36 AM