



File ..DATA\2020\20200930\1121\CPK2020-929-15606.D Tgt Mass (CHM):  
Injection Date : 30 Sep 20 12:10 pm +0800 Seq. Line : 44  
Sample Name : CPK2020-929-15606 Location : P1-A-08  
Acq. Operator : zyj\_1547 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2020\20200930\1121\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2020\20200930\1121\1-POS-3MIN.M  
Catalog No : HY-15253  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

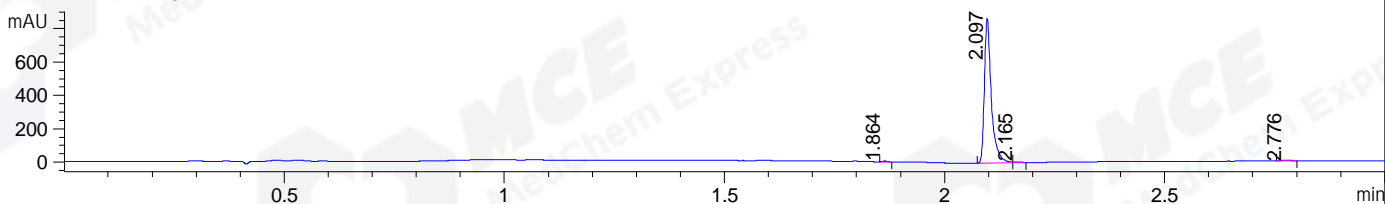


DAD1 C, Sig=254,4 Ref=off

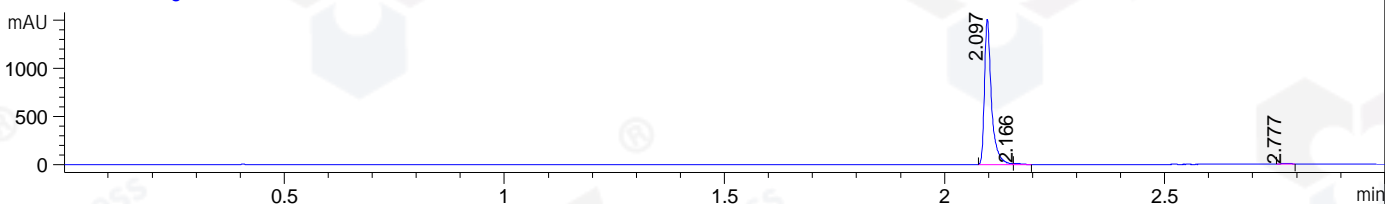

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

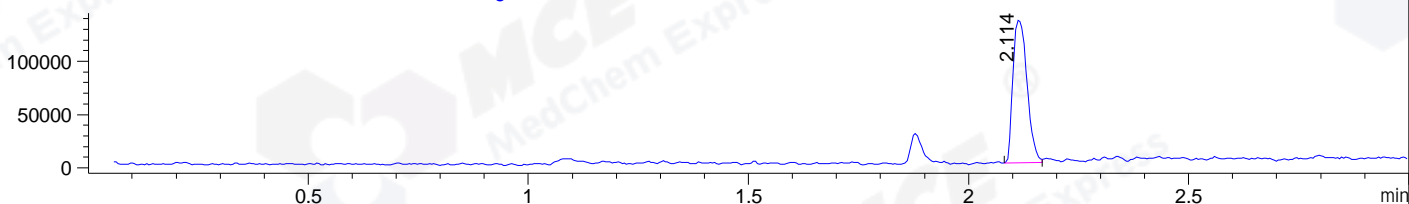

Ion 440, MSD1 440, Target Mass 439 +H Positive, EIC=439.7:440.7

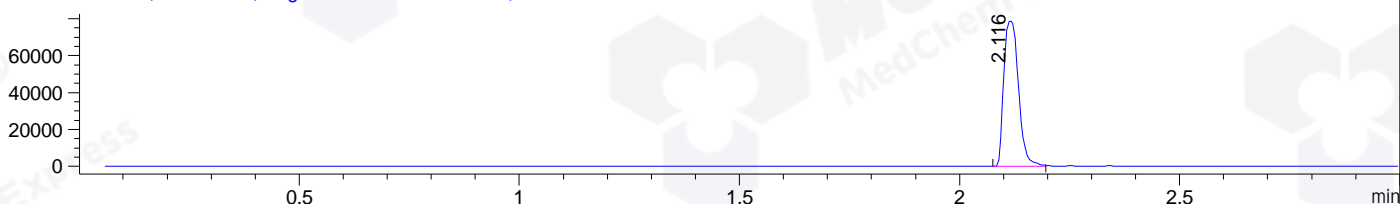

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.86	0.01	3.93	4.80	0.41	288
2.10	0.02	950.15	866.57	98.22	440
2.17	0.02	5.57	5.11	0.58	440
2.78	0.03	7.73	4.98	0.80	ND

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
2.10	0.02	1678.35	1514.71	98.42	440
2.17	0.02	16.52	13.31	0.97	440
2.78	0.02	10.50	7.75	0.62	ND

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.11	0.04	298190.03	134391.66	100.00	440

Ret. Time: 2.11

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

