

File ..1\DATA\2019\20190121\546\BIZ2019-121-WYQ4.D Tgt Mass (CHM):

Injection Date : 21 Jan 19 5:16 pm +0800 Seq. Line : 26

Sample Name : BIZ2019-121-WYQ4 Location : P1-F-02

Acq. Operator : LQ_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190121\546\1-POS-3MIN-1.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190121\546\1-POS-3MIN-1.M

Catalog No : HY-15287A Batch#36994

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-314

Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

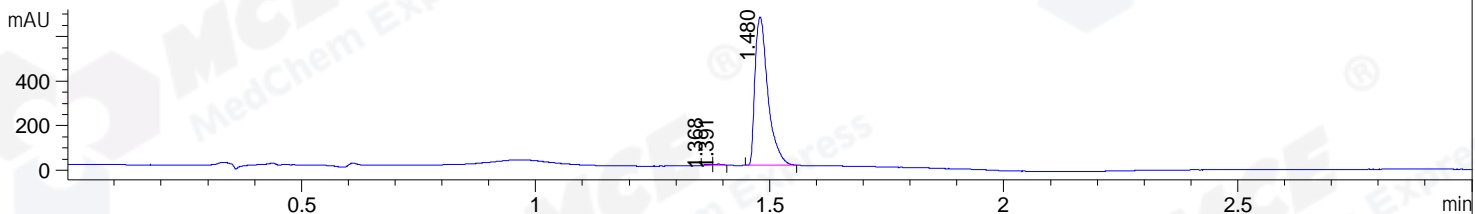


DAD1 C, Sig=254,4 Ref=off

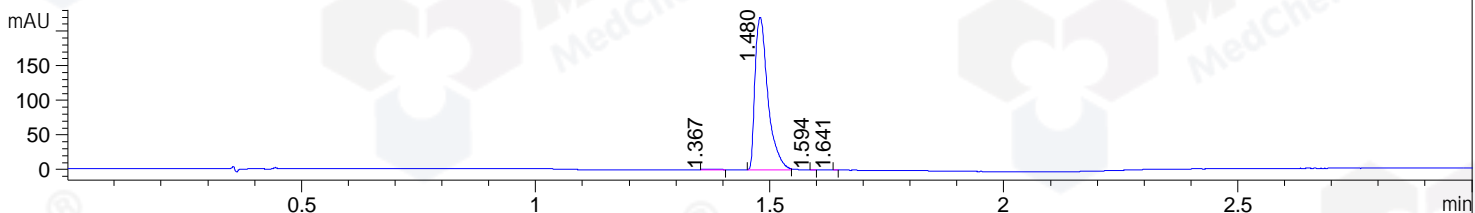

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

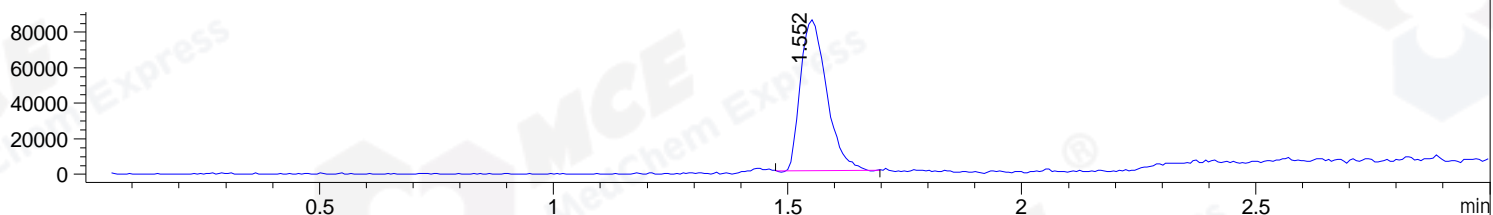

Ion 664.3, MSD1 664.3, Target Mass 663.3 +H Positive, EIC=664:665

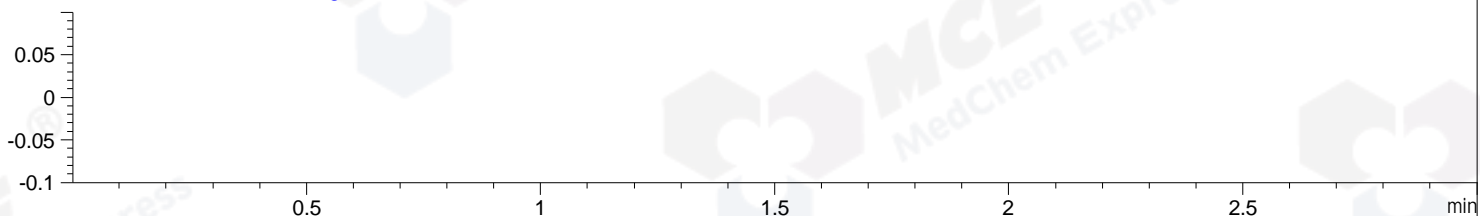

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.37	0.02	5.83	5.57	0.45	ND
1.39	0.02	6.77	5.39	0.53	ND
1.48	0.03	1274.44	665.81	99.02	568

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.37	0.03	1.51	0.80	0.36	ND
1.48	0.03	420.31	220.41	99.61	568
1.59	0.01	0.08	0.17	0.02	568
1.64	0.01	0.04	0.13	0.01	568

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.55	0.06	329959.25	85022.73	100.00	568

Ret. Time: 1.55

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

