



File ..DATA\2020\20200925\1117\CPK2020-925-16010.D Tgt Mass (CHM):
 Injection Date : 25 Sep 20 6:13 pm +0800 Seq. Line : 108
 Sample Name : CPK2020-925-16010 Location : P1-D-03
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200925\1117\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200925\1117\1-POS-3MIN.M
 Catalog No : HY-15317
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

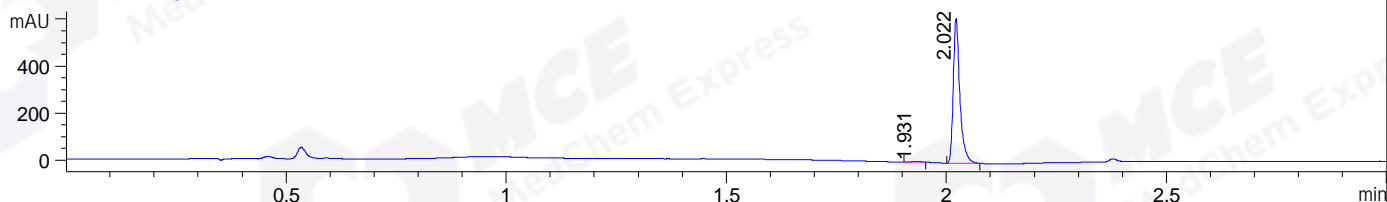


DAD1 C, Sig=254,4 Ref=off

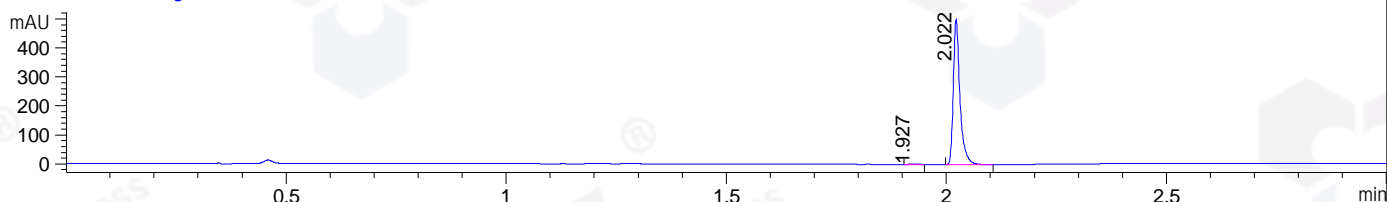

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

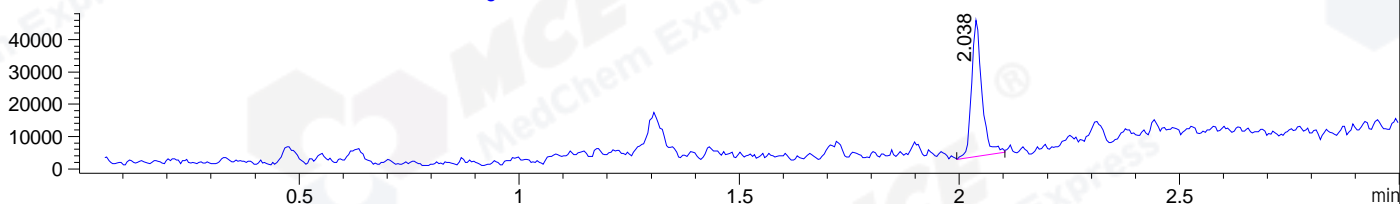

Ion 360, MSD1 360, Target Mass 359 +H Positive, EIC=359.7:360.7

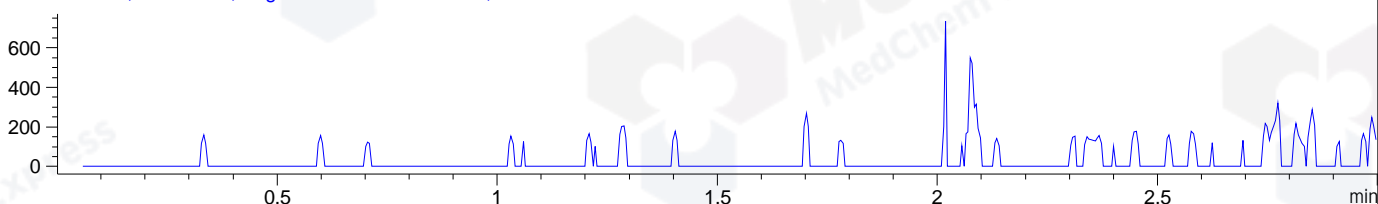

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.93	0.03	3.72	2.02	0.57	ND
2.02	0.02	644.37	615.32	99.43	363

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.93	0.02	0.88	0.62	0.17	ND
2.02	0.02	529.90	501.83	99.83	363

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.04	0.02	69305.74	42484.19	100.00	363

Ret. Time: 2.04

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

