
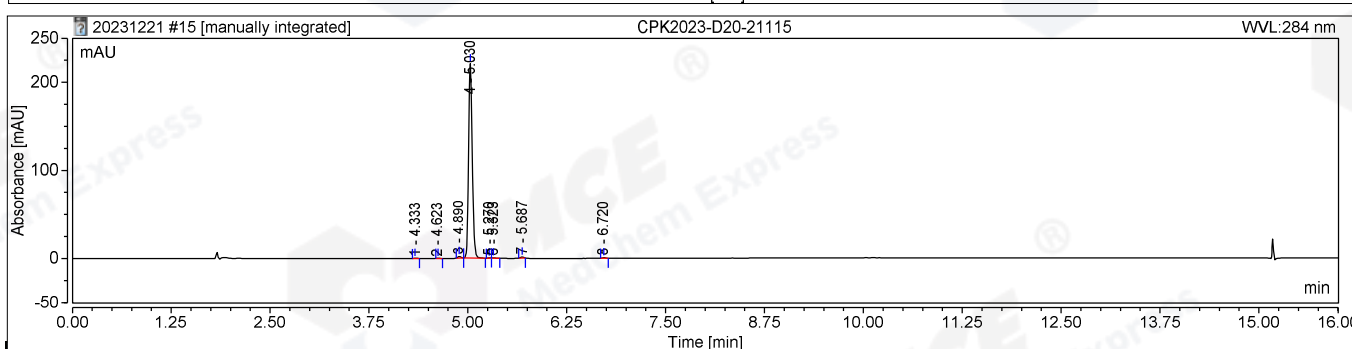


## Chromatogram and Results

Injection Details		
CAS NO.:	520-26-3	Run Time (min): 16.00
Vial Number:	BE3	Injection Volume: 5.00
Injection Type:	Unknown	Channel: EXT284NM
Comment:	A-RP-1283	Wavelength: n.a.
Instrument Method:	10-90A	Bandwidth: n.a.
Processing Method:	3D Quantitative	Dilution Factor: 1.0000
Injection Date/Time:	21/Dec/23 14:52	seq.update_operator: hll
seq.creation_operator:	hll	instMeth.creation_operator: sy
injection.dilution_factor:	1.0000	rdf.update_operator: hll
instMeth.creation_time:	16/Jul/2022 09:02	
chm.rawpath:	chrom://hy442/DATA2/Instrument Data/202312/20231221.seq/332.smp/EXT284NM.channel/EXT284NM.chm	

### Chromatogram

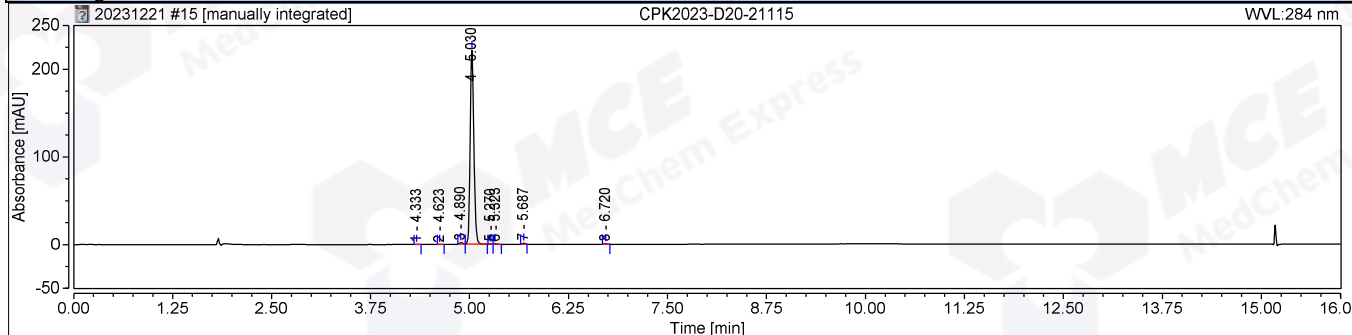

Integration Results								
No.	Peak Name	Retention Time min	Area mAU*s	Height mAU	Relative Area %	Resolution (SM)	Asymmetry (EP)	Plates (EP)
1		4.333	0.5534	0.215	0.0774	4.61	1.29	59946
2		4.623	0.2789	0.114	0.0390	4.11	1.24	74046
3		4.890	5.2609	1.886	0.7354	1.75	1.23	63858
4		5.030	701.5635	220.761	98.0647	3.21	1.18	58698
5		5.270	0.8345	0.306	0.1166	0.73	n.a.	n.a.
6		5.323	1.7296	0.490	0.2418	4.81	n.a.	n.a.
7		5.687	3.3339	1.287	0.4660	15.15	0.99	98110
8		6.720	1.8539	0.628	0.2591	n.a.	1.15	105623
<b>Total:</b>			<b>715.4086</b>	<b>225.688</b>	<b>100.000</b>		<b>7</b>	