



File ..1\DATA\2018\20180910\379\BIZ2018-907-WYQ1.D Tgt Mass (CHM):

Injection Date : 10 Sep 18 1:14 pm +0800 Seq. Line : 21  
 Sample Name : BIZ2018-907-WYQ1 Location : P2-A-02  
 Acq. Operator : LQ\_1052 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2018\20180910\379\1-POS-3MIN-1.M  
 Analysis Method : D:\CHEM32\1\DATA\2018\20180910\379\1-POS-3MIN-1.M  
 Catalog No : HY-15346 Batch#32606 BY DMSO A-RP-314  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-314  
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

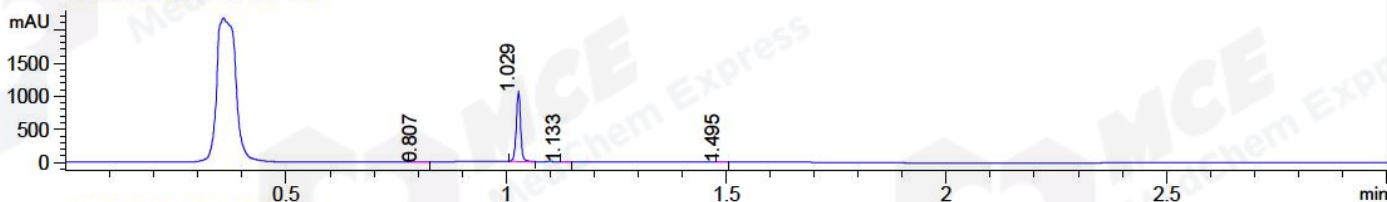


DAD1 C, Sig=254,4 Ref=off

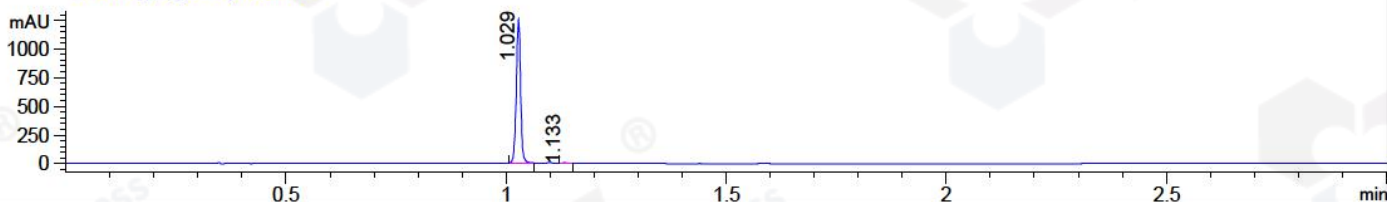

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

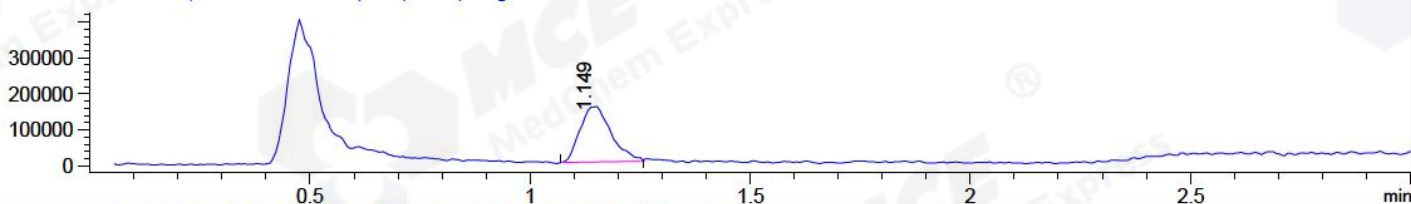

Ion 481.2, MSD1 481.2, Target Mass 480.2 +H Positive, EIC=480.9:481.9

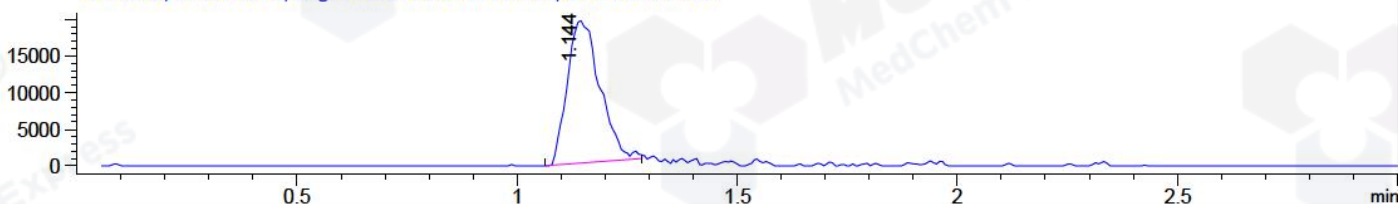

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.81	0.03	3.69	2.17	0.49	157
1.03	0.01	739.23	1059.10	98.91	157
1.13	0.01	2.62	3.93	0.35	241
1.49	0.02	1.80	1.91	0.24	157

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.03	0.01	879.26	1263.48	99.65	157
1.13	0.01	3.09	4.47	0.35	241

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.15	0.07	758002.25	155403.31	100.00	241

Ret. Time: 1.15

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

