

File ..\DATA\2020\20200104\803\CPK2020-103-23448.D Tgt Mass (CHM):

Injection Date : 4 Jan 20 10:39 am +0800 Seq. Line : 18

Sample Name : CPK2020-103-23448 Location : PI-A-09

Acq. Operator : ZJ\_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2020\20200104\803\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200104\803\1-POS-3MIN.M

Catalog No : HY-15415 Batch# 23448

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

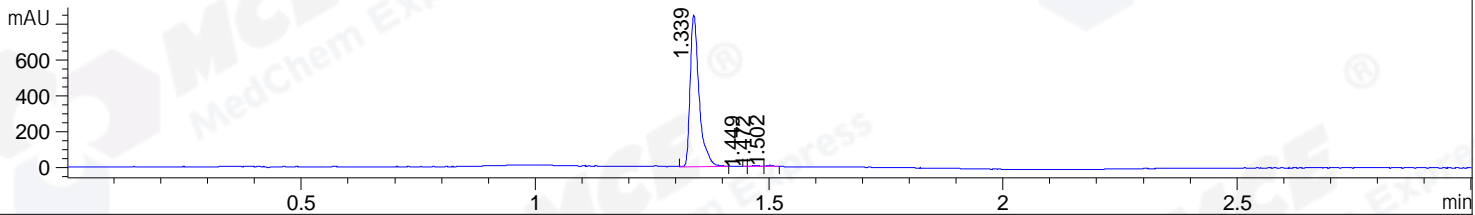


DAD1 C, Sig=254,4 Ref=off

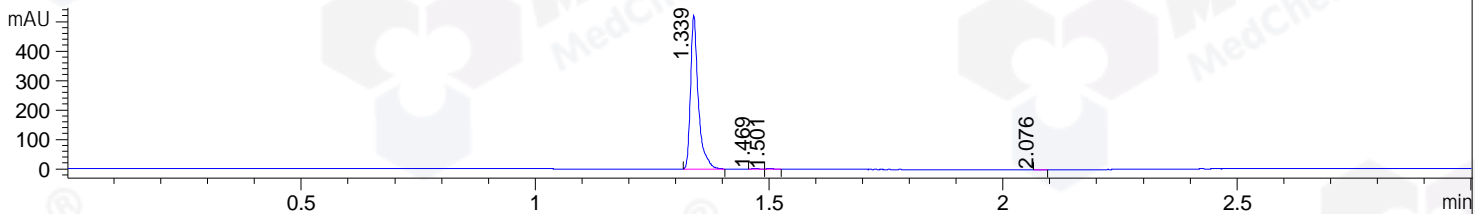

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

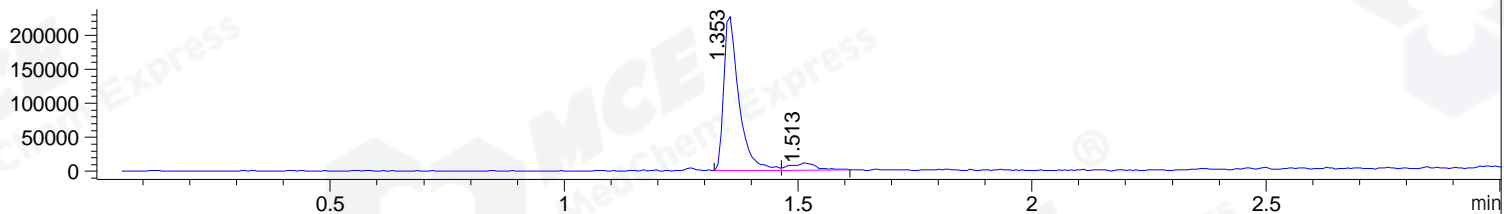

Ion 428, MSD1 428, Target Mass 427 +H Positive, EIC=427.7:428.7

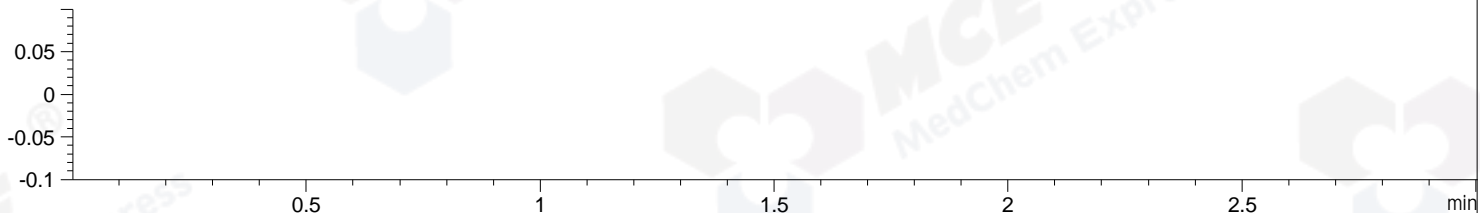

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.34	0.02	1129.22	847.79	98.82	332
1.45	0.01	0.57	1.70	0.05	332
1.47	0.02	5.95	4.46	0.52	332
1.50	0.02	7.01	7.36	0.61	452

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.34	0.02	603.67	522.94	99.20	332
1.47	0.02	2.10	2.27	0.34	332
1.50	0.02	1.98	2.13	0.33	452
2.08	0.01	0.82	0.99	0.13	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.35	0.03	512394.69	228955.13	92.38	332

1.51      0.06      42247.36      11254.21      7.62      332

Ret. Time: 1.35

<<<< POSITIVE SPECTRA >>>>

ES-API Positive



Ret. Time: 1.51

ES-API Positive

