

File ..DATA\2020\20200610\988\CPK2020-609-13909-.D Tgt Mass (CHM):

Injection Date : 10 Jun 20 6:57 pm +0800 Seq. Line : 117

Sample Name : CPK2020-609-13909 Location : PL-B-04

Acq. Operator : ZJ\_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 0.3 ul

Acq. Method : D:\Chem32\1\data\2020\20200610\988\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200610\988\1-POS-3MIN.M

Catalog No : HY-15527

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

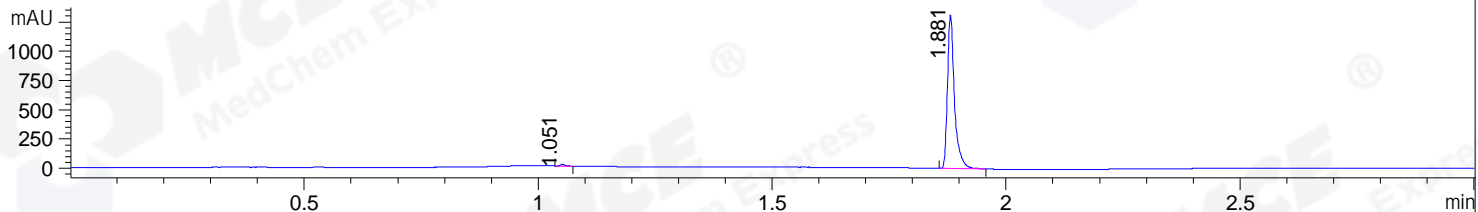


DAD1 C, Sig=254,4 Ref=off

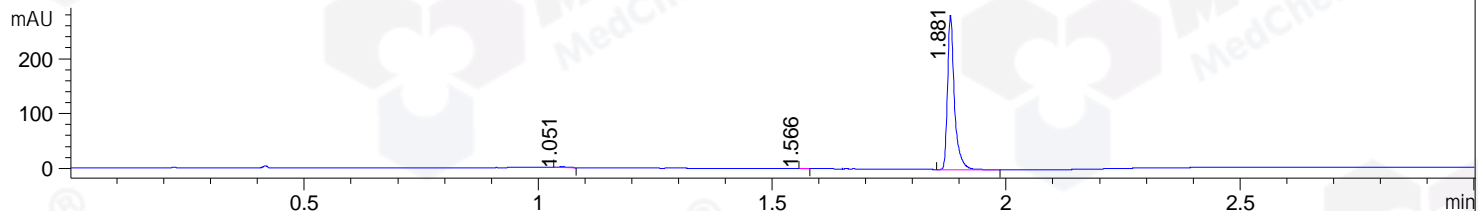

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

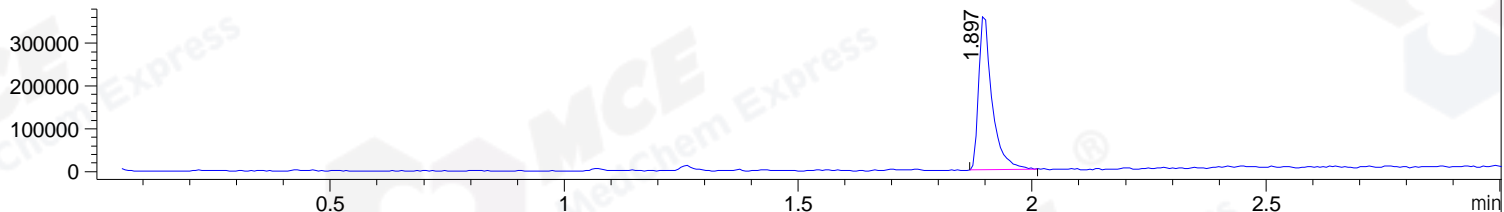

Ion 402, MSD1 402, Target Mass 401 +H Positive, EIC=401.7:402.7

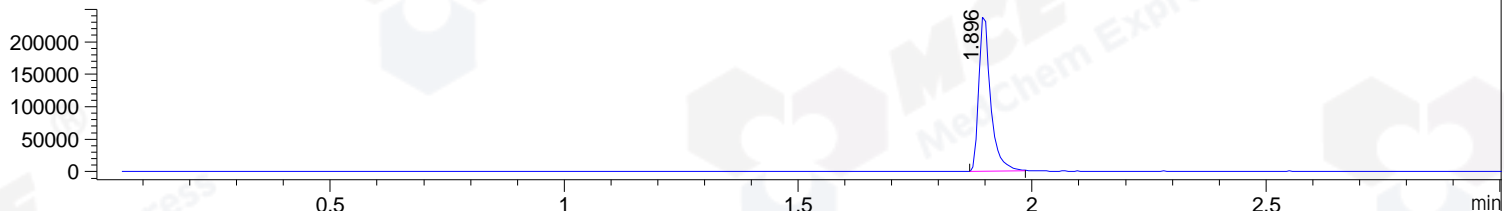

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.05	0.01	11.54	13.11	0.83	361
1.88	0.02	1373.85	1314.37	99.17	402

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.05	0.02	1.74	1.46	0.59	361
1.57	0.01	0.43	0.63	0.15	ND
1.88	0.02	292.00	282.18	99.26	402

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.90	0.03	725788.88	371323.84	100.00	402

Ret. Time: 1.90

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

