


File ..ta\2018\20180821\20180821 2\SQS5831-003-2.D Tgt Mass (CHM):
 Injection Date : 21 Aug 18 11:10 am +0800 Seq. Line : 33
 Sample Name : SQS5831-003-2 Location : P1-B-10
 Acq. Operator : SYSTEM Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\LCMS03\Data\2018\20180821\20180821 2\1-POS-3MIN.M
 Analysis Method : D:\LCMS03\Data\2018\20180821\20180821 2\1-POS-3MIN.M
 Catalog No : HY-15534 Batch#32270
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-186
 Oven Temperature : 45C

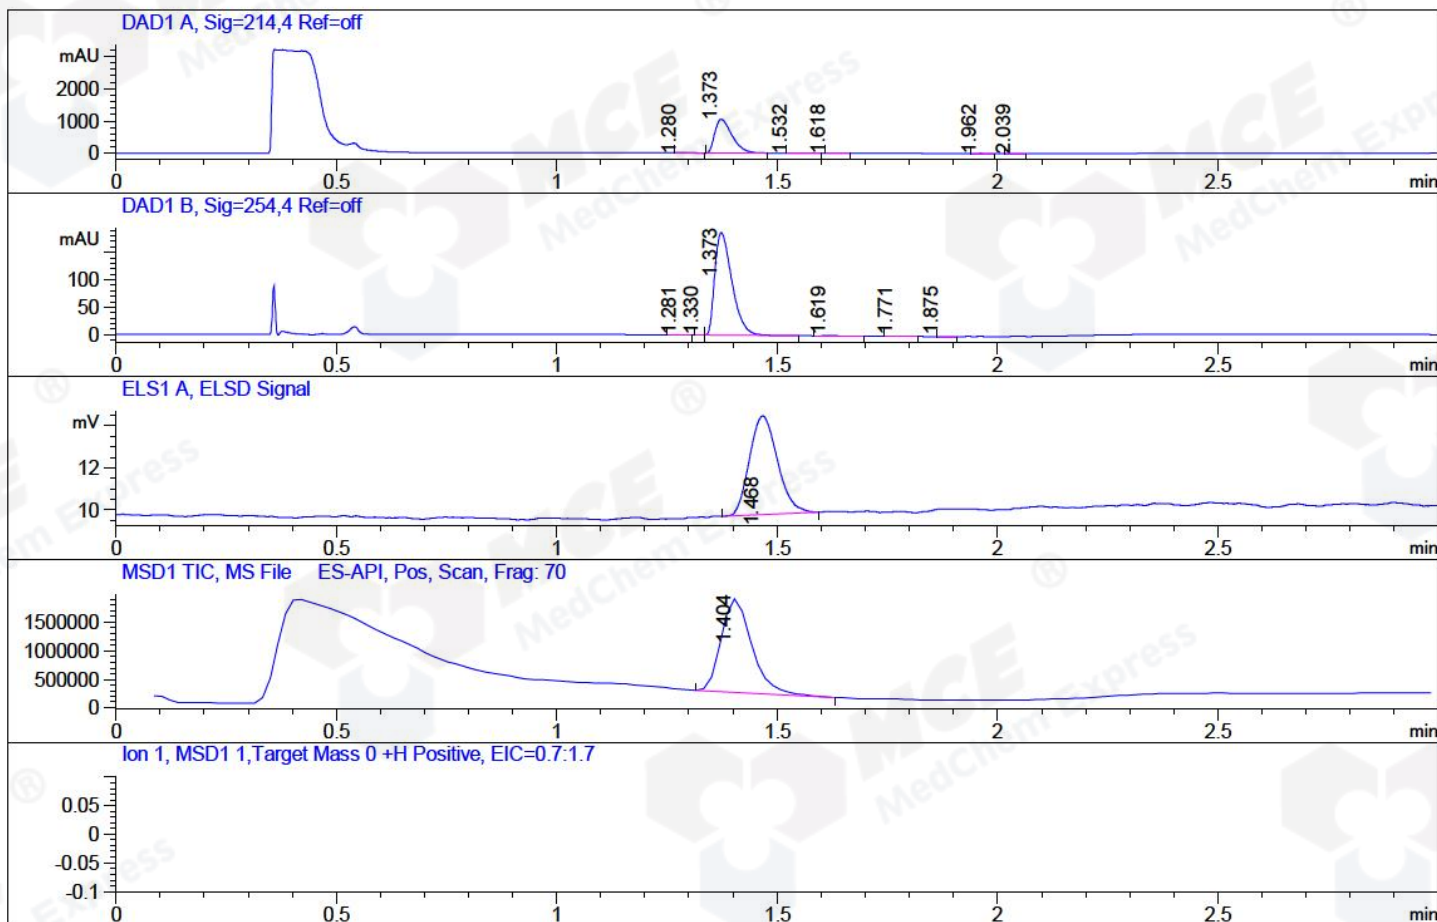

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.28	0.03	3.31	1.23	0.12	157
1.37	0.04	2806.34	1040.37	99.55	525
1.53	0.03	2.01	1.15	0.07	157
1.62	0.03	0.94	0.47	0.03	130
1.96	0.02	5.66	4.35	0.20	130
2.04	0.02	0.71	0.50	0.03	130

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.28	0.03	0.37	0.20	0.07	157
1.33	0.01	0.21	0.25	0.04	157
1.37	0.04	504.09	186.21	99.46	525
1.62	0.03	1.39	0.72	0.27	130
1.77	0.03	0.62	0.30	0.12	130
1.87	0.02	0.15	0.11	0.03	130

Integration Results for ELS1 A, ELSD Signal


RetTim	Width	Area	Height	Area%	MS (+)
1.47	0.07	20.77	4.70	100.00	525

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.40	0.07	7926845.00	1636799.50	100.00	525

Ret. Time: 1.40

<<<< POSITIVE SPECTRA >>>>

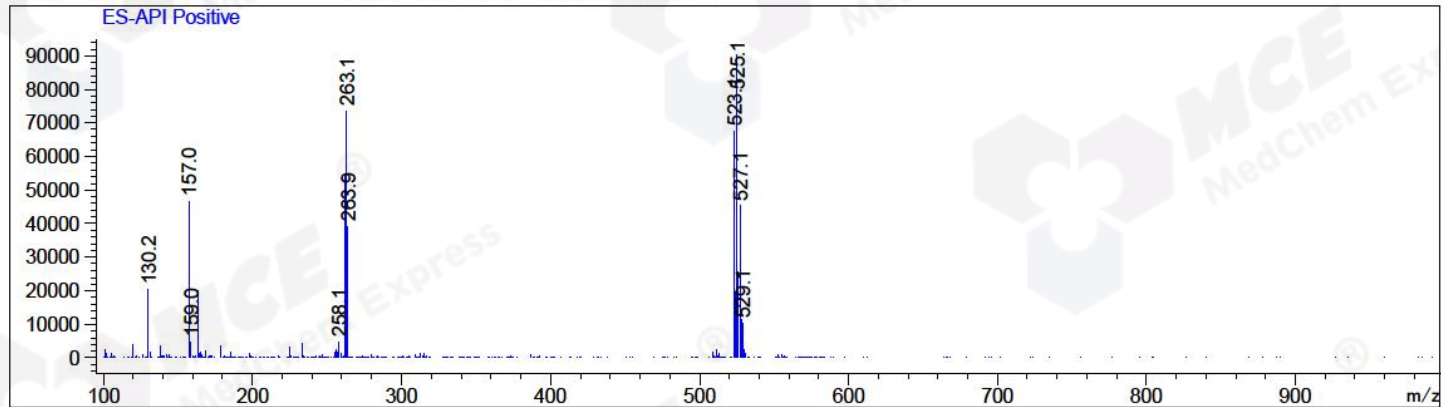

*** End of Report ***