
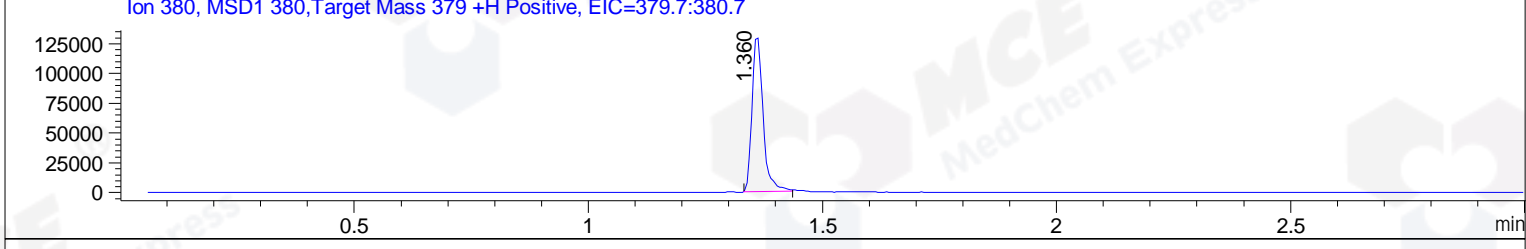
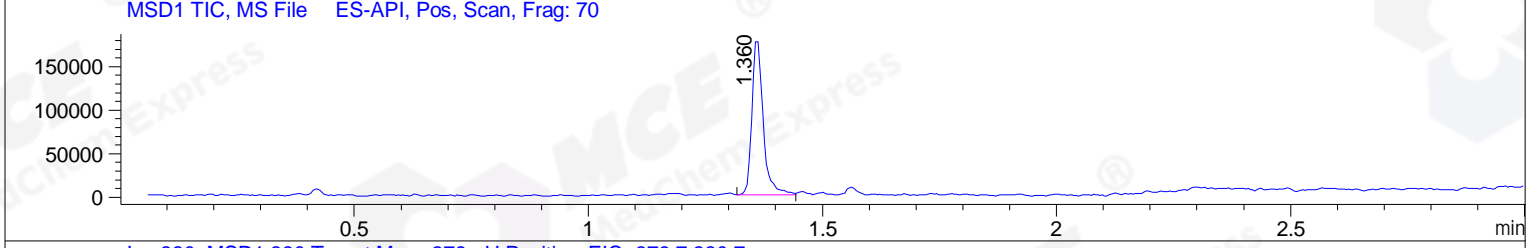
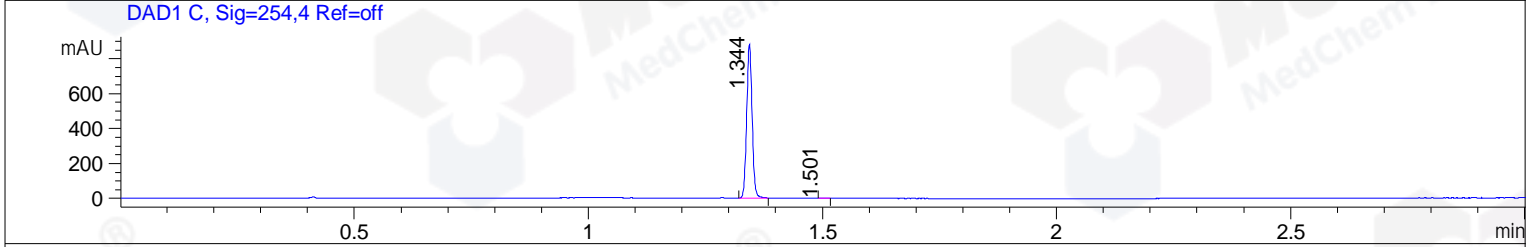


File ..DATA\2020\20200730\1058\CPK2020-730-27160.D Tgt Mass (CHM):
 Injection Date : 30 Jul 20 4:34 pm +0800 Seq. Line : 91
 Sample Name : CPK2020-730-27160 Location : P1-C-02
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200730\1058\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200730\1058\1-POS-3MIN.M
 Catalog No : HY-15604
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-314
 Oven Temperature : 45C

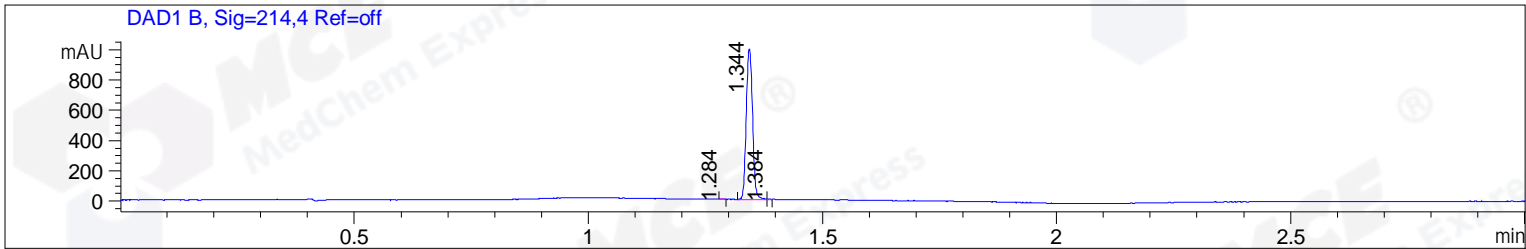

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.28	0.01	1.16	2.41	0.12	ND
1.34	0.02	930.22	994.85	99.78	380
1.38	0.01	0.93	2.65	0.10	380

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.34	0.01	708.97	881.80	99.90	380
1.50	0.01	0.71	0.82	0.10	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.36	0.03	300660.97	179838.23	100.00	380

Ret. Time: 1.36

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

