



File ..DATA\2020\20201030\1141\CPK2020-029-09017.D Tgt Mass (CHM):  
Injection Date : 30 Oct 20 9:02 pm +0800 Seq. Line : 149  
Sample Name : CPK2020-029-09017 Location : P1-E-02  
Acq. Operator : zyj\_1547 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2020\20201030\1141\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2020\20201030\1141\1-POS-3MIN.M  
Catalog No : HY-15609  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

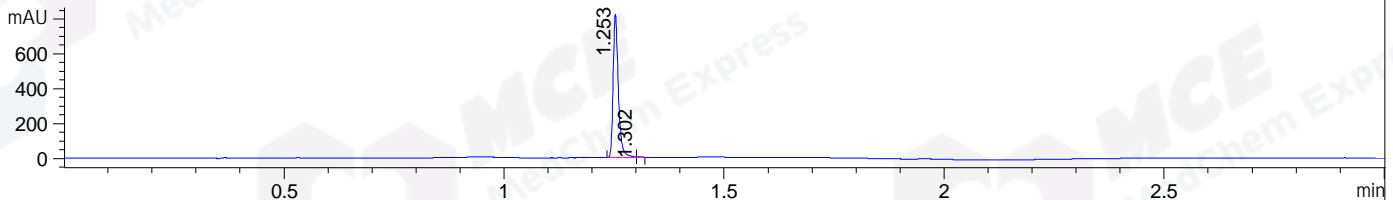


DAD1 C, Sig=254,4 Ref=off

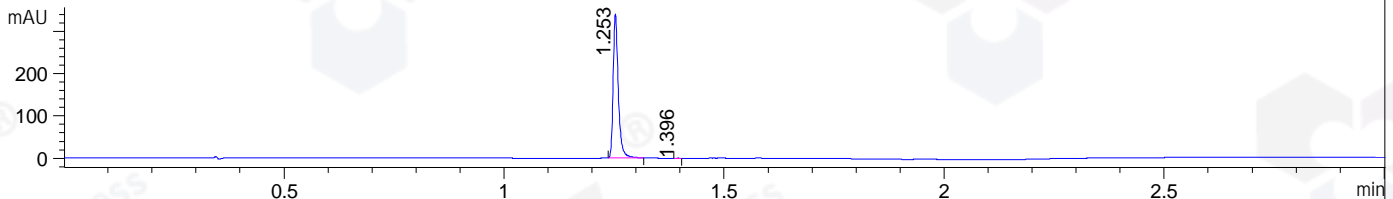

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

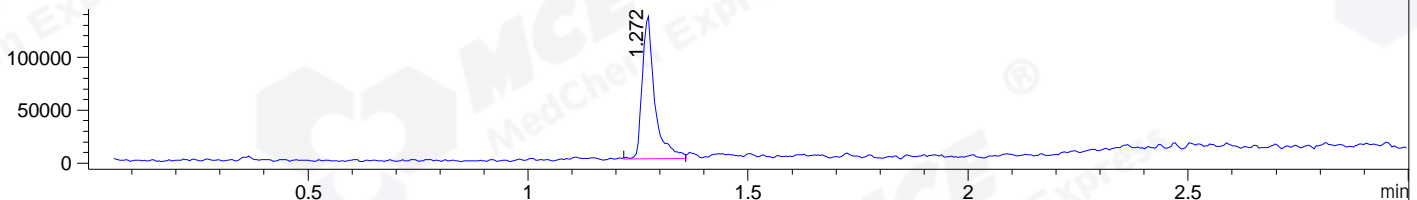

Ion 449, MSD1 449, Target Mass 448 +H Positive, EIC=448.7:449.7

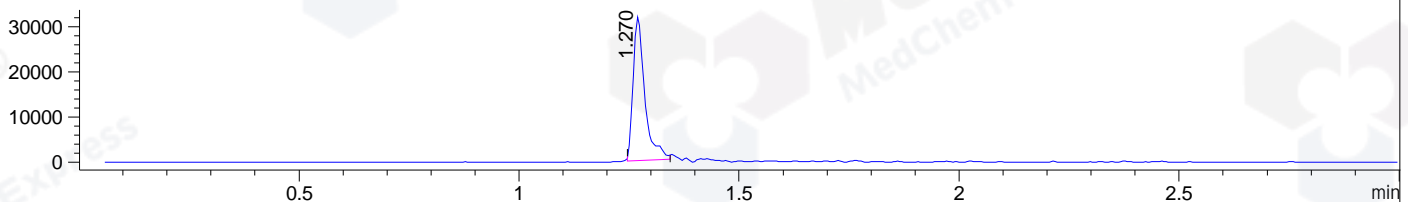

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.01	679.57	819.16	99.79	449
1.30	0.01	1.42	2.31	0.21	449

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.01	277.55	341.19	99.96	449
1.40	0.01	0.10	0.18	0.04	ND

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.27	0.03	265938.22	136182.94	100.00	449

Ret. Time: 1.27

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

