

File ..1\DATA\2019\20190927\720\BIZ2019-926-SCH5.D Tgt Mass (CHM):

Injection Date : 27 Sep 19 11:03 am +0800 Seq. Line : 28

Sample Name : BIZ2019-926-SCH5 Location : PI-A-04

Acq. Operator : bgd_1571 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190927\720\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2019\20190927\720\1-POS-3MIN.M

Catalog No : HY-15615A Batch#46291

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-433

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

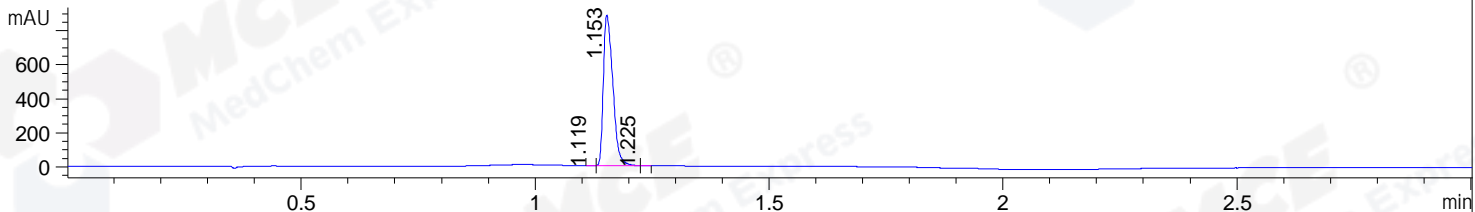


DAD1 C, Sig=254,4 Ref=off

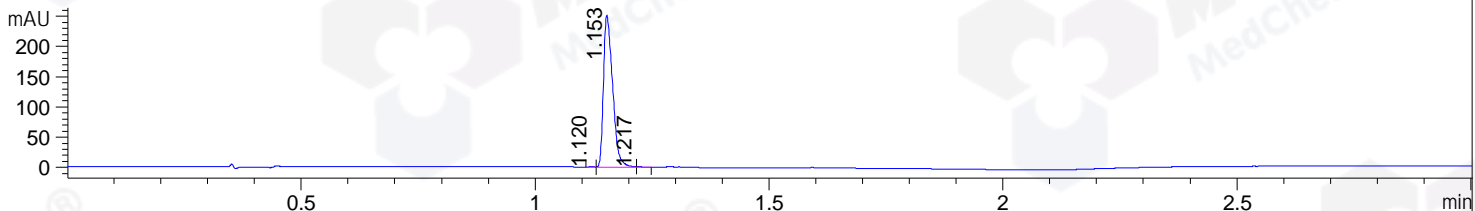

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

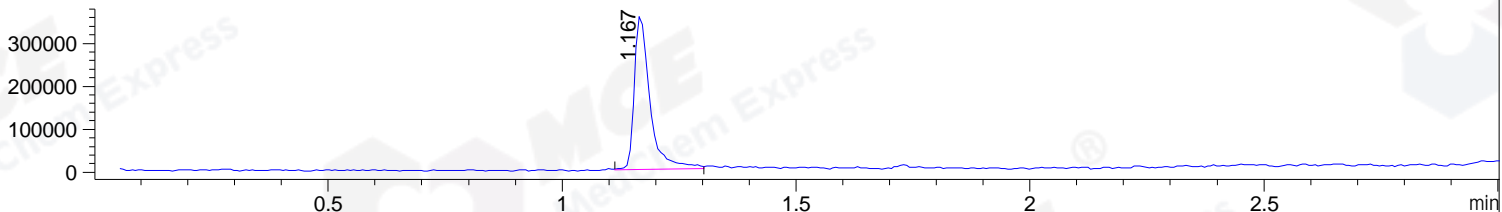

Ion 387.21, MSD1 387.21, Target Mass 386.21 +H Positive, EIC=386.91:387.91

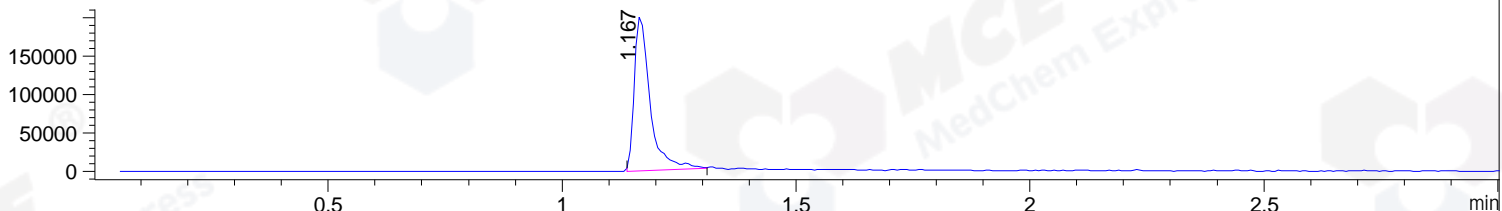

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.12	0.02	1.34	1.43	0.11	373
1.15	0.02	1242.89	886.16	99.80	387
1.23	0.01	1.17	1.60	0.09	387

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.12	0.02	0.44	0.47	0.13	373
1.15	0.02	338.88	251.39	99.72	387
1.22	0.01	0.50	0.62	0.15	387

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.04	840189.44	360376.84	100.00	387

Ret. Time: 1.17

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

