



File ..2\MONITOR\HY-CYQ2736-037-1-01891-LCMSA033.D Tgt Mass (EZX):  
 Injection Date : 14 Aug 15 10:25 am +0800 Seq. Line : 0  
 Sample Name : HY-CYQ2736-037-1 Location : P1-B-03  
 Acq. Operator : A02-MONITOR Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 2 ul  
 Acq. Method : D:\METHODS\2-NEG-MON-2.8MIN.M  
 Analysis Method : D:\METHODS\2-NEG-MON-2.8MIN.M  
 Catalog No : HY-15677 Batch#17445  
 Method Info : Mobile Phase : A:water(10mM NH4HCO3) B:ACN  
 Gradient:5%B for 0.2min,increase to 95%B within 1.5min,95%B for 1.3min,back to 5%  
 within 0.01min  
 Flow Rate :1.6ml/min  
 Column : XBridge C18, 50\*4.6mm,3.5um  
 Column Temperature:50C


\*ADC1 A, ELSD

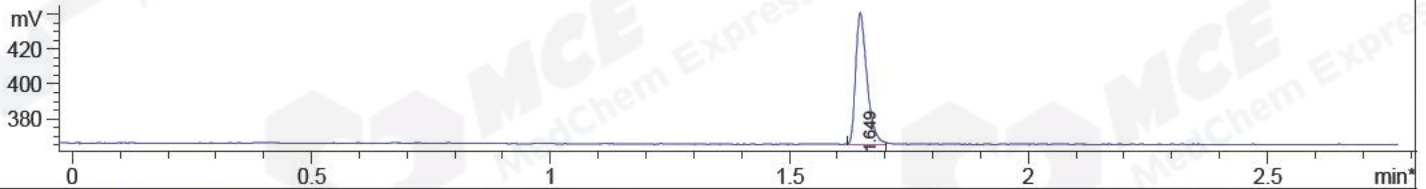


\*DAD1 A, Sig=214,4 Ref=off

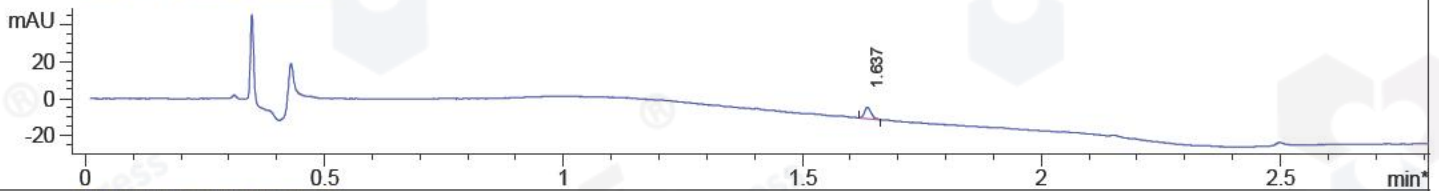

\*DAD1 B, Sig=254,4 Ref=off

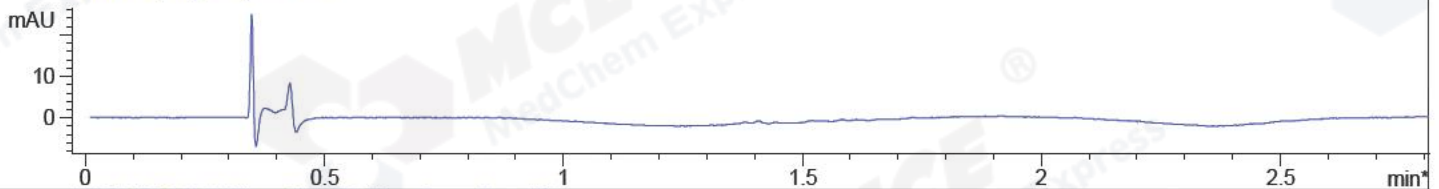

\*MSD1 TIC, MS File ES-API, Neg, Scan, Frag: 70

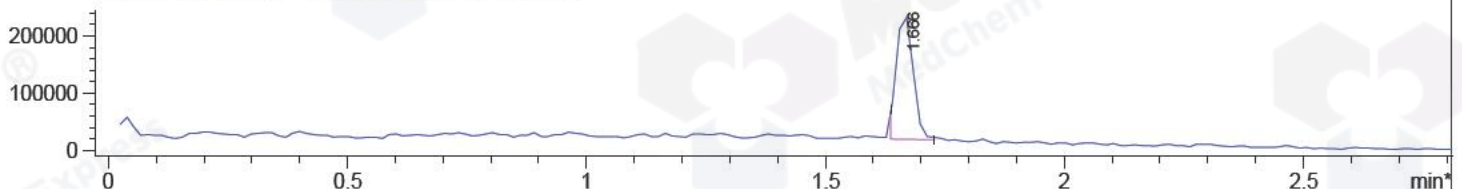

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
1.65	0.02	123.08	75.29	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.64	0.02	5.96	6.11	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%

Ret. Time: 1.67

<<<< NEGATIVE SPECTRA >>>>

