


20 CPK2019-D24-11670**Catalog No: HY-15741 Batch#11670 A-RP-520 JLW**

Sample Name:	CPK2019-D24-11670	Injection Volume:	2.0
Vial Number:	GC1	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	210
Control Program:	30-90A 210NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2019-12-25 19:57	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

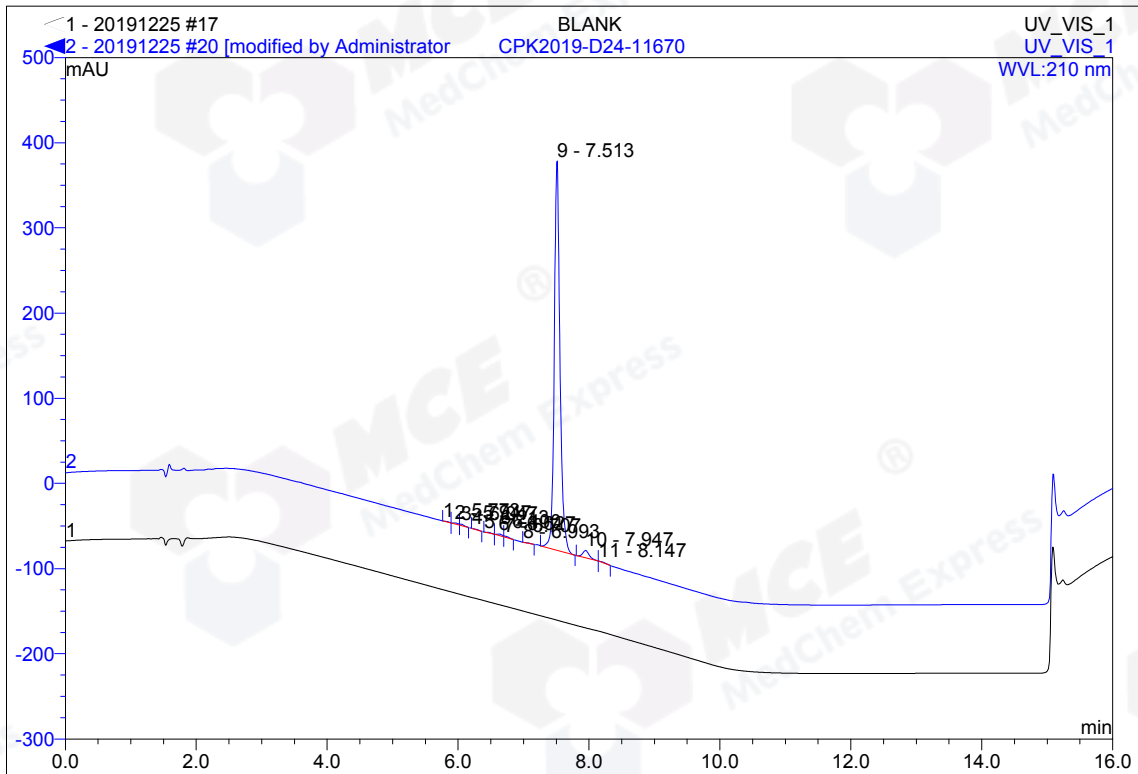

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	5.77	n.a.	0.014	0.028	0.06	n.a.	BMb*
2	5.95	n.a.	1.052	0.114	0.23	n.a.	bM *
3	6.05	n.a.	1.614	0.118	0.24	n.a.	MB*
4	6.21	n.a.	0.015	0.033	0.07	n.a.	BMB*
5	6.40	n.a.	0.007	0.043	0.09	n.a.	BMb*
6	6.63	n.a.	1.798	0.182	0.37	n.a.	bM *
7	6.71	n.a.	1.146	0.116	0.24	n.a.	MB*
8	6.99	n.a.	0.004	0.031	0.06	n.a.	BMB*
9	7.51	n.a.	457.001	46.968	96.47	n.a.	BMB*
10	7.95	n.a.	8.631	0.979	2.01	n.a.	BMb*
11	8.15	n.a.	0.065	0.073	0.15	n.a.	bMB*
Total:			471.348	48.686	100.00	0.000	