



File ..DATA\2021\20210302\1290\CPK2021-226-17871.D Tgt Mass (CHM):
Injection Date : 2 Mar 21 1:29 pm +0800 Seq. Line : 51
Sample Name : CPK2021-226-17871 Location : P1-A-03
Acq. Operator : yrz_1364 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2021\20210302\1290\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2021\20210302\1290\1-POS-3MIN.M
CAS NO. : 1493764-08-1
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

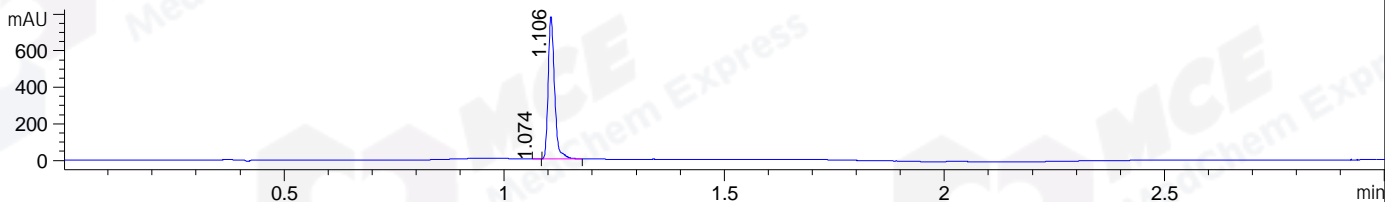


DAD1 C, Sig=254,4 Ref=off

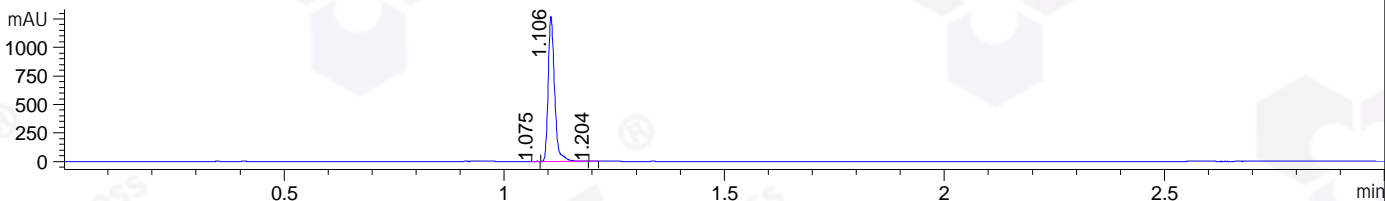

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

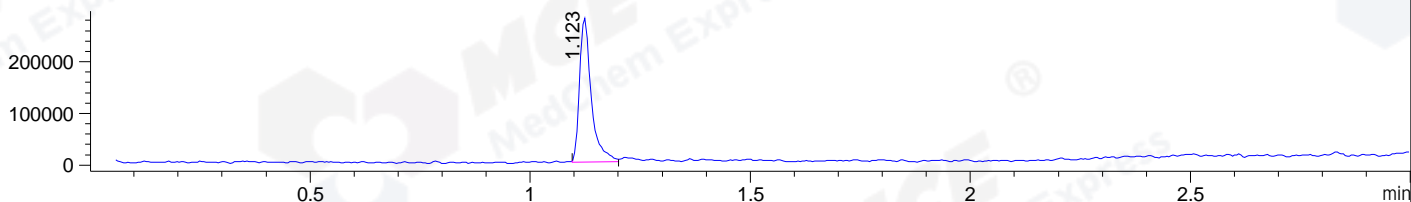

Ion 464, MSD1 464, Target Mass 463 +H Positive, EIC=463.7:464.7

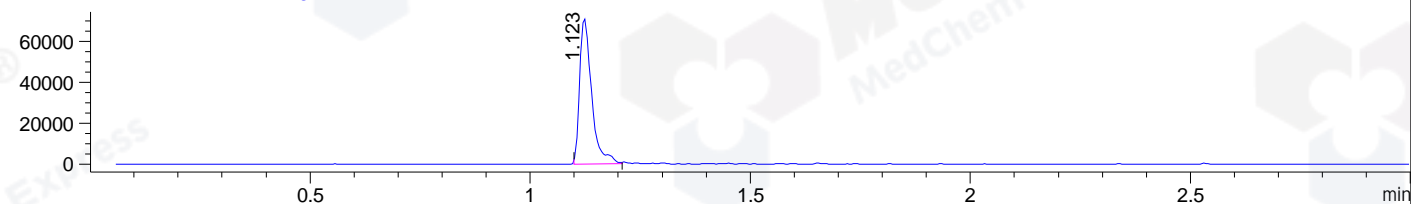

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.07	0.01	0.71	0.86	0.09	ND
1.11	0.02	790.98	780.17	99.91	233

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.07	0.01	0.66	1.05	0.05	ND
1.11	0.02	1294.21	1273.99	99.89	233
1.20	0.01	0.82	1.21	0.06	233

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.12	0.03	516317.56	280006.59	100.00	233

Ret. Time: 1.12

<<<< POSITIVE SPECTRA >>>>

