


3 CPK2019-927-11386**Catalog No: HY-15881 Batch# 11386 A-RP-427 LY**

Sample Name:	CPK2019-927-11386	Injection Volume:	5.0
Vial Number:	BC6	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	210
Control Program:	10-90A 210NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2019-9-27 15:15	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

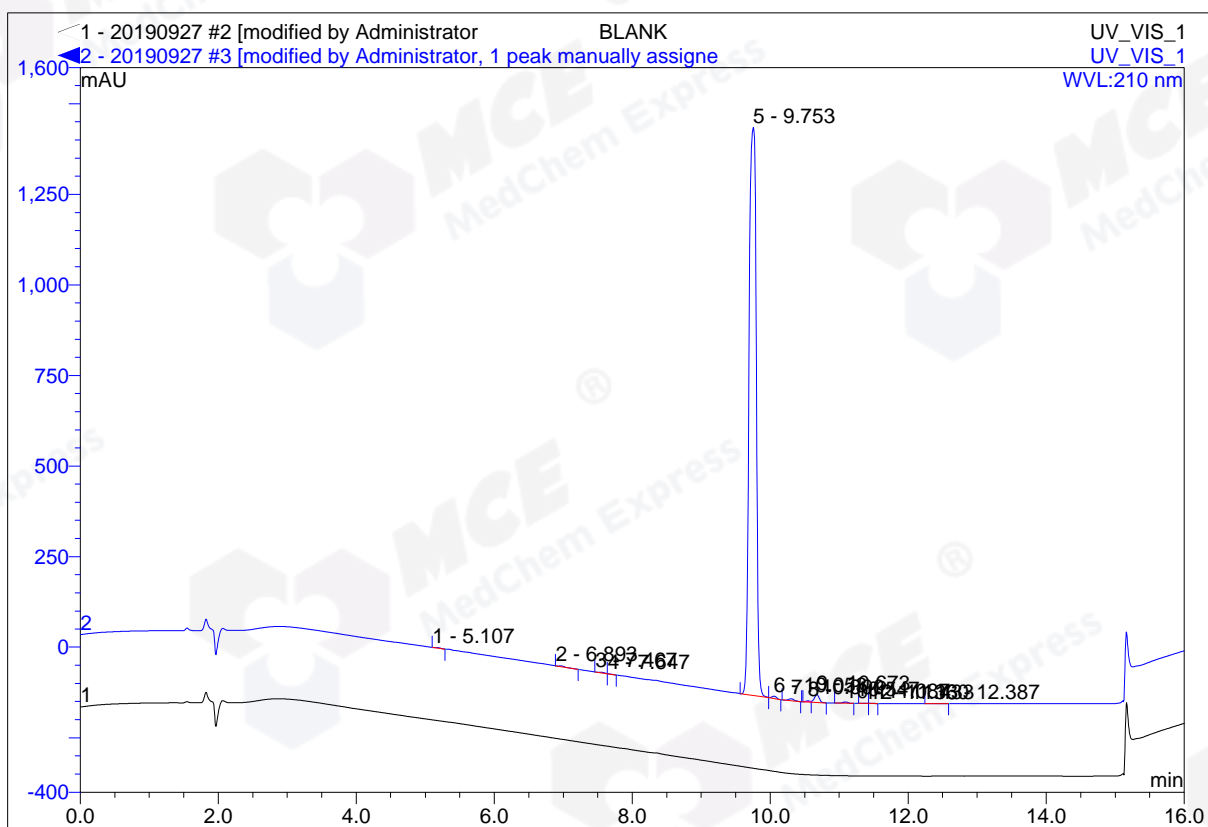

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	5.11	n.a.	0.004	0.101	0.05	n.a.	BMB
2	6.89	n.a.	0.008	0.159	0.08	n.a.	BMB
3	7.47	n.a.	0.006	0.137	0.07	n.a.	BM
4	7.65	n.a.	0.363	0.029	0.02	n.a.	MB
5	9.75	n.a.	1567.657	188.137	98.06	n.a.	BMB
6	10.05	n.a.	6.326	0.475	0.25	n.a.	bMB
7	10.30	n.a.	5.567	0.514	0.27	n.a.	BMB
8	10.55	n.a.	1.996	0.118	0.06	n.a.	Ru^
9	10.67	n.a.	21.666	1.873	0.98	n.a.	BMB
10	11.09	n.a.	3.255	0.288	0.15	n.a.	BMB
11	11.36	n.a.	0.122	0.011	0.01	n.a.	BM *
12	11.43	n.a.	0.066	0.006	0.00	n.a.	MB*
13	12.39	n.a.	0.127	0.019	0.01	n.a.	BMB*
Total:			1607.163	191.866	100.00	0.000	