



File ..\DATA\2020\20200107\806\CPK2020-106-12049.D Tgt Mass (CHM):
Injection Date : 7 Jan 20 2:57 pm +0800 Seq. Line : 79
Sample Name : CPK2020-106-12049 Location : P1-A-06
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20200107\806\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20200107\806\1-POS-3MIN.M
Catalog No : HY-15948 Batch#12049
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

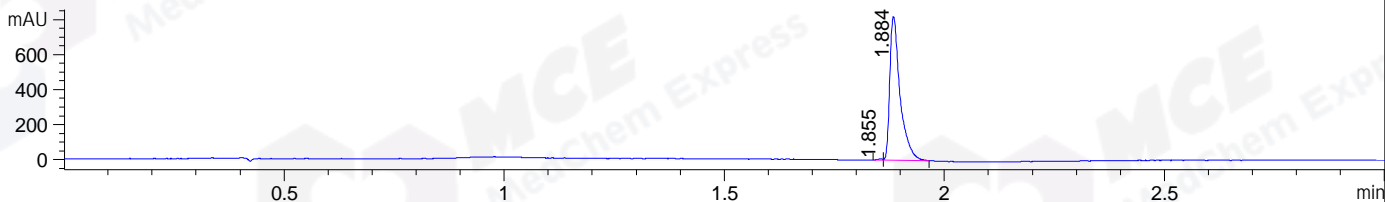


DAD1 C, Sig=254,4 Ref=off

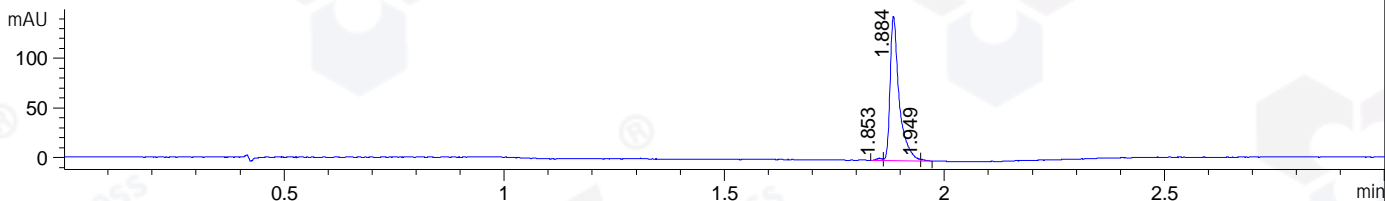

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

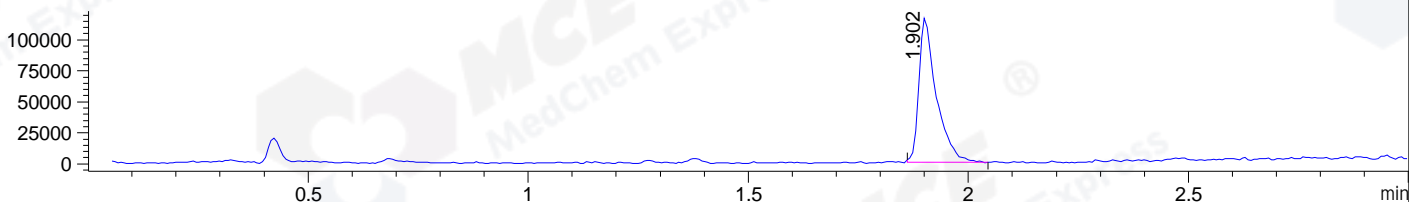

Ion 431, MSD1 431, Target Mass 430 +H Positive, EIC=430.7:431.7

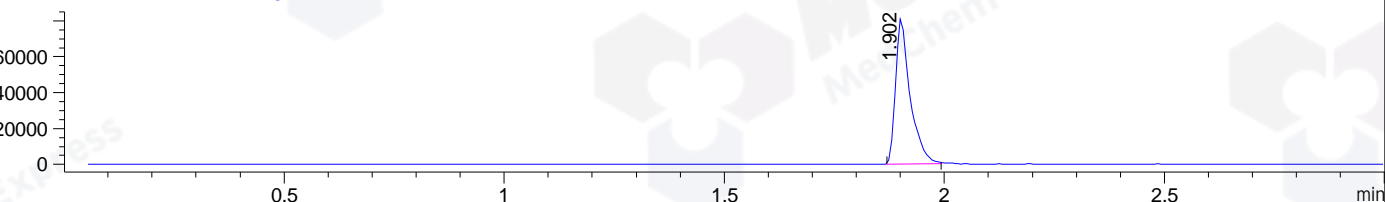

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.85	0.02	6.23	6.81	0.47	ND
1.88	0.03	1329.75	822.44	99.53	431

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.85	0.02	1.89	2.05	0.91	ND
1.88	0.02	206.22	145.56	98.67	431
1.95	0.01	0.88	1.29	0.42	431

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.90	0.04	320469.38	116551.87	100.00	431

Ret. Time: 1.90

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

