



File ..\DATA\2020\20200902\1095\BIZ2020-901-WLQ3.D Tgt Mass (CHM):
 Injection Date : 2 Sep 20 12:47 pm +0800 Seq. Line : 4
 Sample Name : BIZ2020-901-WLQ3 Location : P1-A-07
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200902\1095\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200902\1095\1-POS-3MIN.M
 Catalog No : HY-15975
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

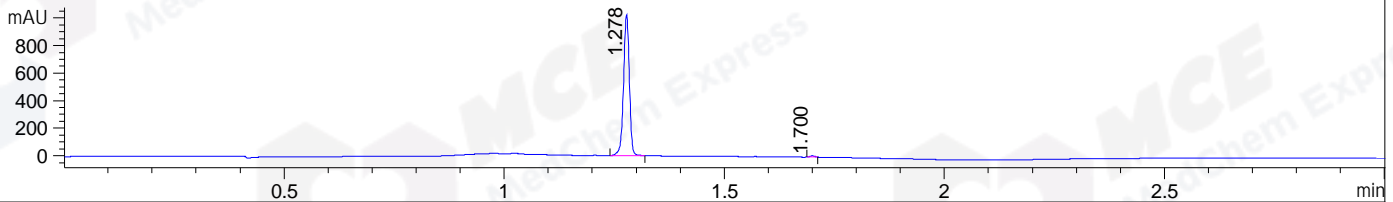


DAD1 C, Sig=254,4 Ref=off

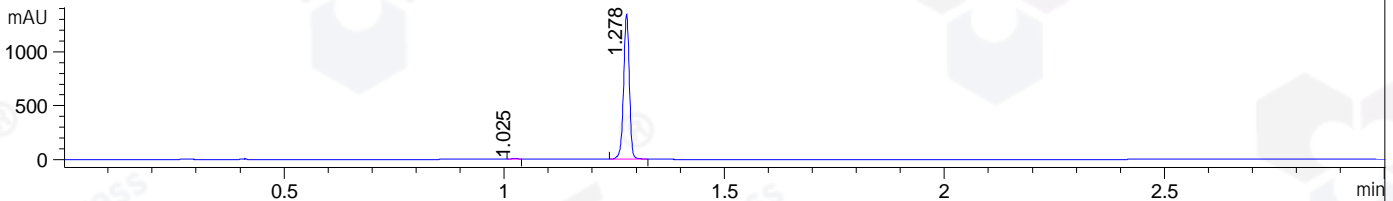

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

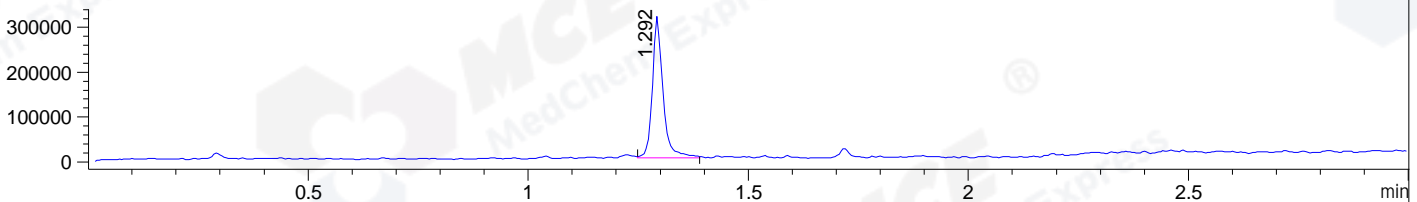

Ion 428, MSD1 428, Target Mass 427 +H Positive, EIC=427.7:428.7

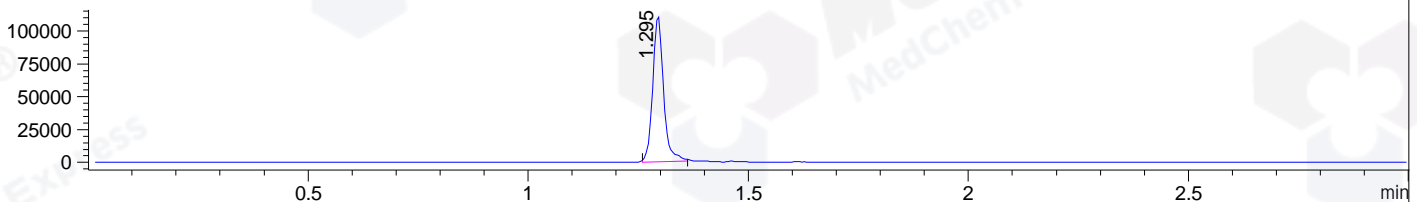

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.28	0.02	941.59	1025.61	99.28	428
1.70	0.01	6.80	9.28	0.72	611

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.02	0.01	6.76	7.63	0.55	303
1.28	0.02	1223.52	1348.29	99.45	428

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.29	0.03	528638.00	316856.88	100.00	428

Ret. Time: 1.29

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

