



File ..DATA\2020\20200703\1025\CPK2020-622-26506.D Tgt Mass (CHM):
 Injection Date : 3 Jul 20 9:06 am +0800 Seq. Line : 5
 Sample Name : CPK2020-622-26506 Location : P1-D-08
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.3 ul
 Acq. Method : D:\Chem32\1\data\2020\20200703\1025\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200703\1025\1-POS-3MIN.M
 Catalog No : HY-15979A
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

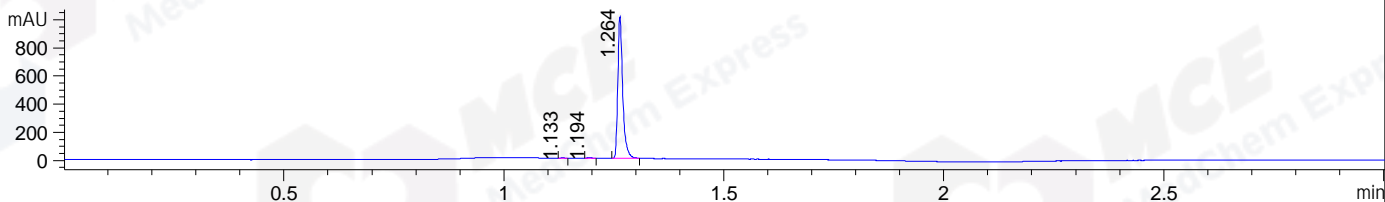


DAD1 C, Sig=254,4 Ref=off

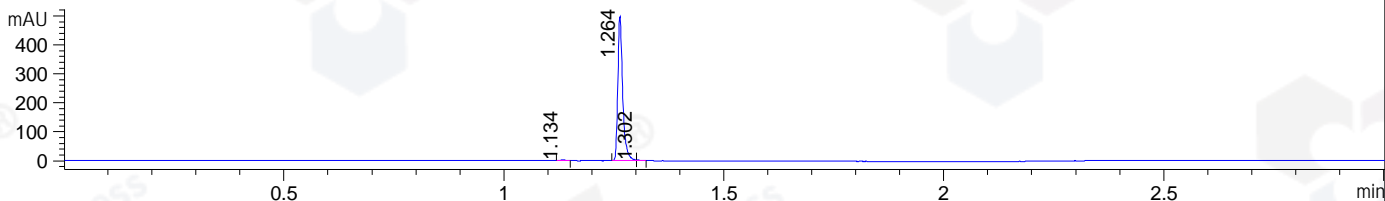

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

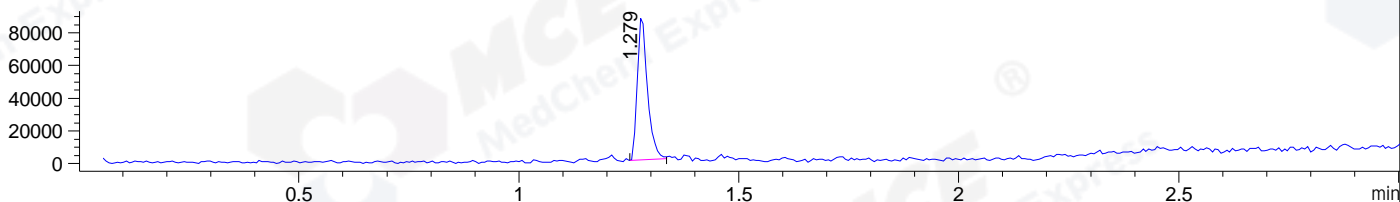

Ion 446, MSD1 446, Target Mass 445 +H Positive, EIC=445.7:446.7

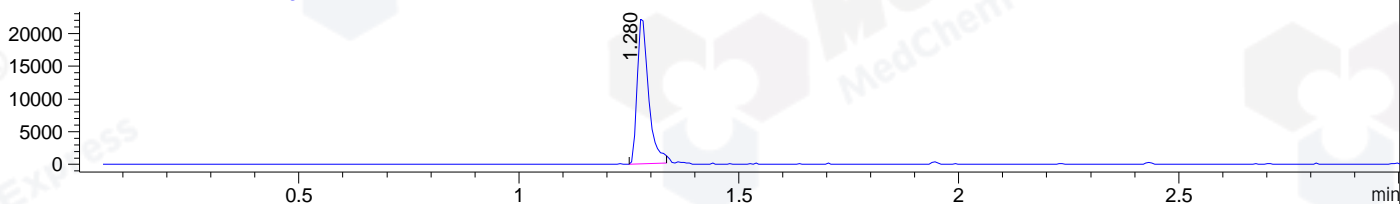

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.01	1.48	2.34	0.19	ND
1.19	0.01	3.70	4.82	0.47	ND
1.26	0.01	783.02	1009.12	99.34	448

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.13	0.01	2.41	3.09	0.62	ND
1.26	0.01	385.46	499.65	99.01	448
1.30	0.01	1.44	2.10	0.37	446

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.28	0.02	141129.30	89639.89	100.00	448

Ret. Time: 1.28

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

