

File ..00630 2020-06-30 08-28-21\ZHJ7908-056-3_2.D Tgt Mass (CHM):

Injection Date : 30 Jun 20 3:04 pm +0800 Seq. Line : 85

Sample Name : ZHJ7908-056-3 Location : P1-D-01

Acq. Operator : SYSTEM Inj : 1

Spec. Reported : MS Integration Inj Volume : 0.08 ul

Acq. Method : D:\LCMS03\Data\20200630\20200630 2020-06-30 08-28-21\1-POS-UPLC5.0MIN(0.8ML)

Analysis Method : D:\LCMS03\Data\20200630\20200630 2020-06-30 08-28-21\1-POS-UPLC5.0MIN(0.8ML)

Catalog No : HY-16293

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 3 min

Flow Rate :0.8ml/min


Column :Poroshell 120 EC- C18, 2.1*50mm,1.9um A-RP-530

Oven Temperature : 45C

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

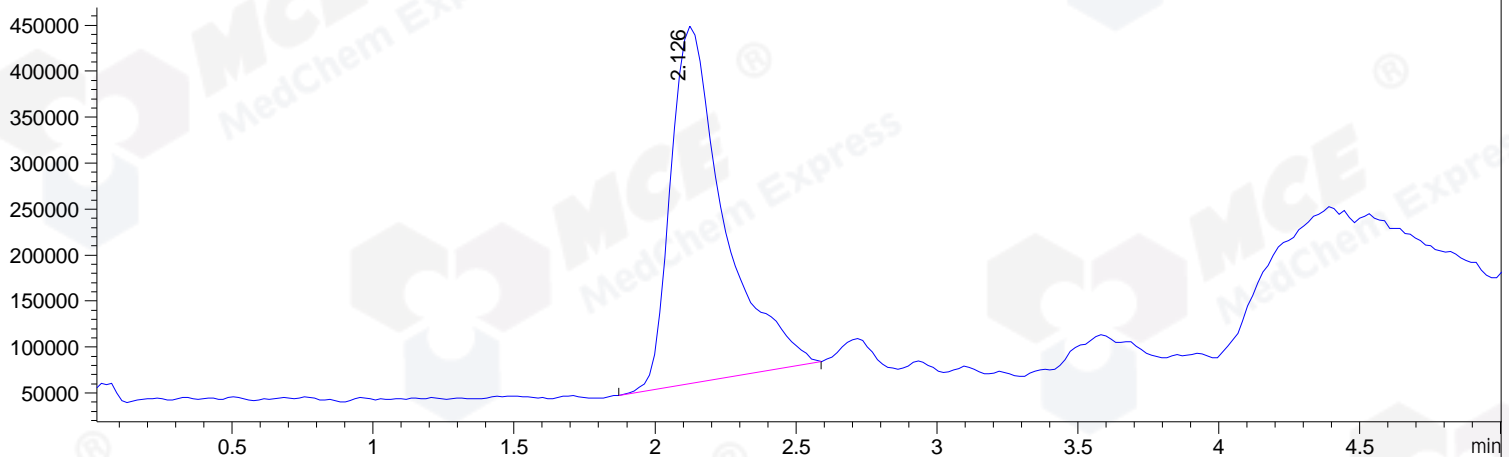

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7:1.7

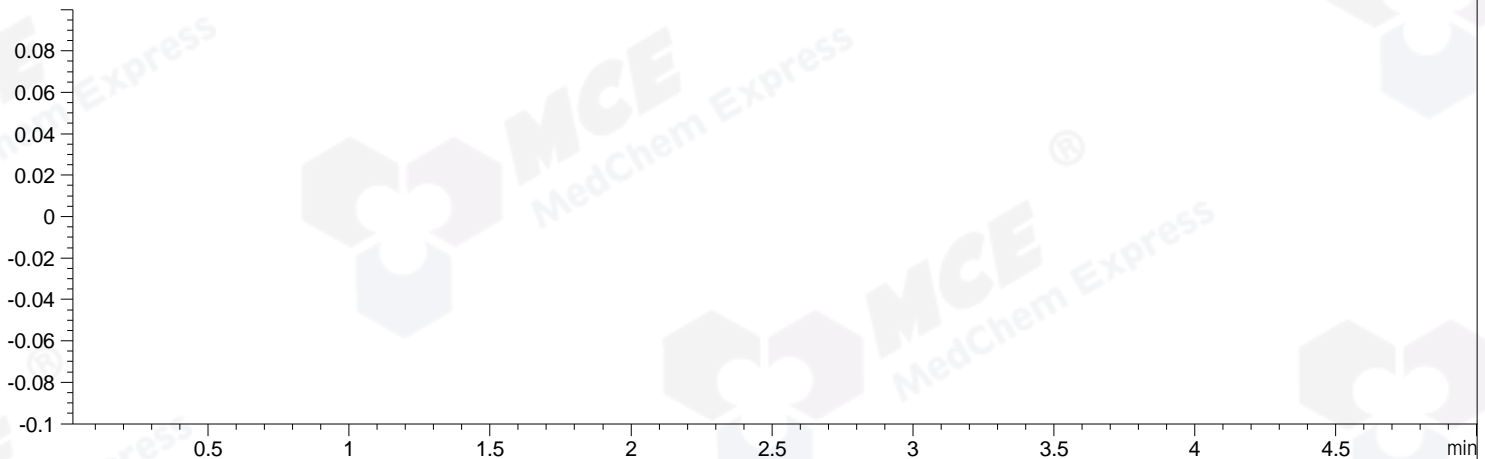


Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
2.13	0.19	5121136.00	389005.34	100.00	384

Ret. Time: 2.13

<<<< POSITIVE SPECTRA >>>>

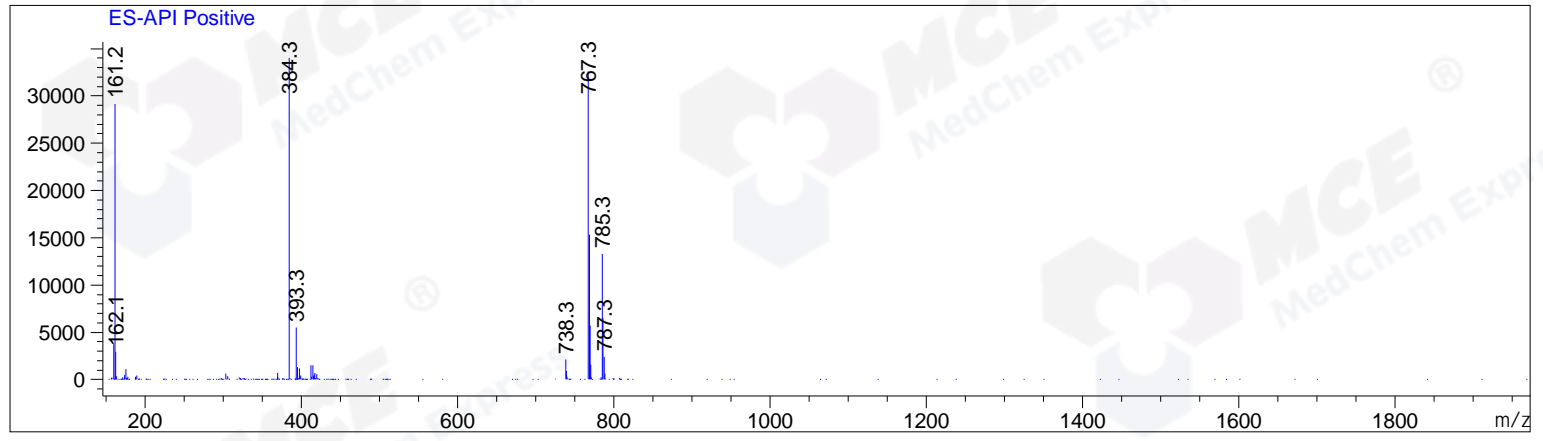

*** End of Report ***