

File ..DATA\2020\20200629\1019\CPK2020-628-07640.D Tgt Mass (CHM):

Injection Date : 29 Jun 20 12:23 pm +0800 Seq. Line : 43

Sample Name : CPK2020-628-07640 Location : PL-B-08

Acq. Operator : ZJ_1432 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2020\20200629\1019\1-POS-3MIN.M

Analysis Method : D:\CHEM32\1\DATA\2020\20200629\1019\1-POS-3MIN.M

Catalog No : HY-16576

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-607

Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

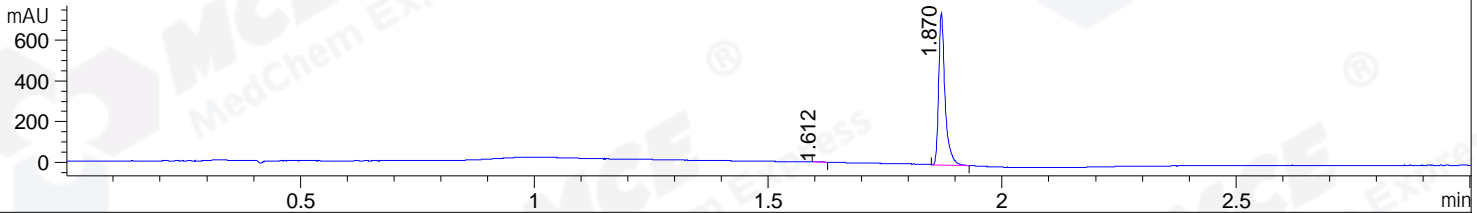


DAD1 C, Sig=254,4 Ref=off

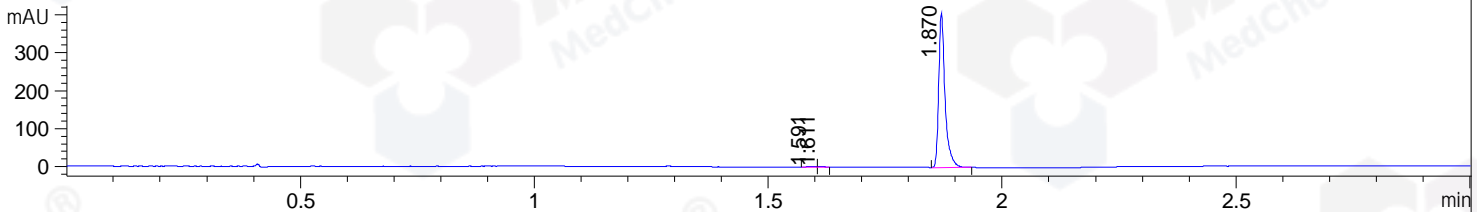

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

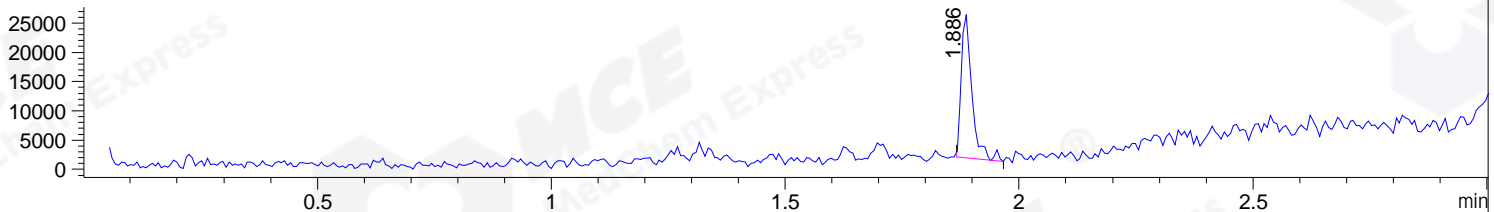

Ion 274, MSD1 274, Target Mass 273 +H Positive, EIC=273.7:274.7

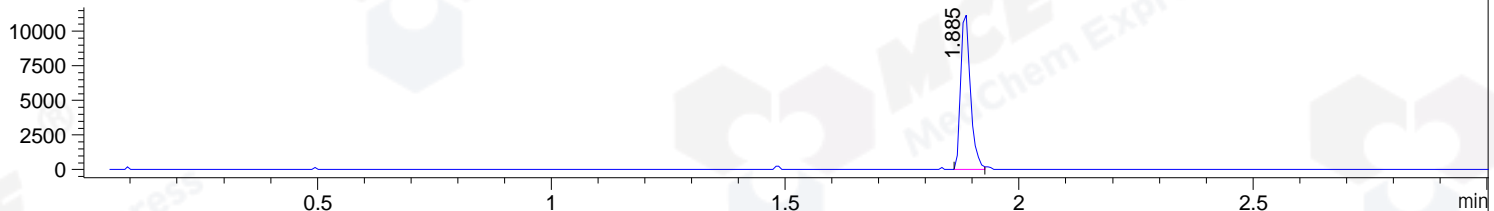

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.61	0.02	1.92	1.71	0.27	ND
1.87	0.02	708.68	749.72	99.73	274

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.59	0.02	1.83	1.35	0.47	ND
1.61	0.01	1.17	1.31	0.30	ND
1.87	0.02	384.80	406.44	99.23	274

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.89	0.02	38140.46	24716.07	100.00	274

Ret. Time: 1.89

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

