



File ..DATA\2021\20210218\1277\CPK2021-218-18821.D Tgt Mass (CHM):  
 Injection Date : 18 Feb 21 8:06 pm +0800 Seq. Line : 25  
 Sample Name : CPK2021-218-18821 Location : P1-A-02  
 Acq. Operator : yrz\_1364 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2021\20210218\1277\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2021\20210218\1277\1-POS-3MIN.M  
 CAS NO. : 1884220-36-3  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

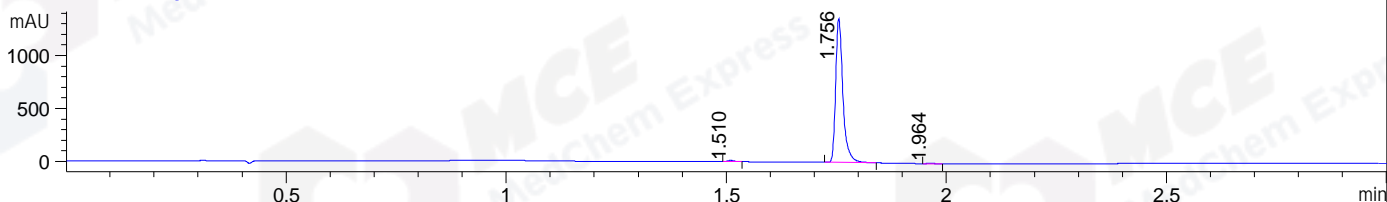


DAD1 C, Sig=254,4 Ref=off

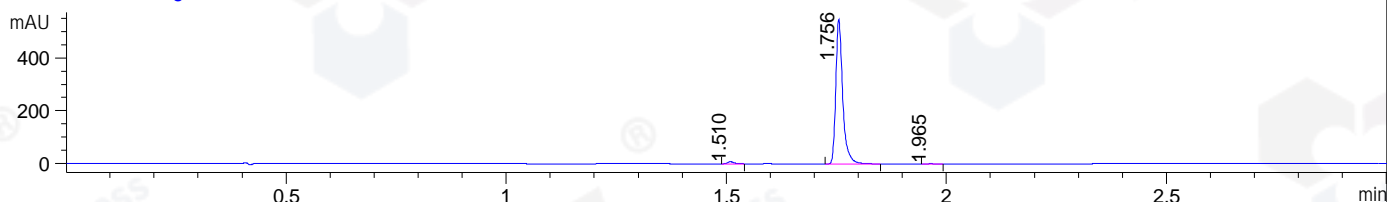

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

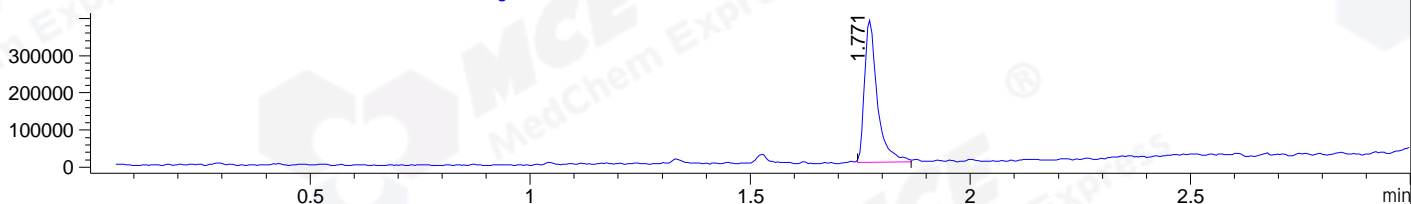

Ion 489, MSD1 489, Target Mass 488 +H Positive, EIC=488.7:489.7

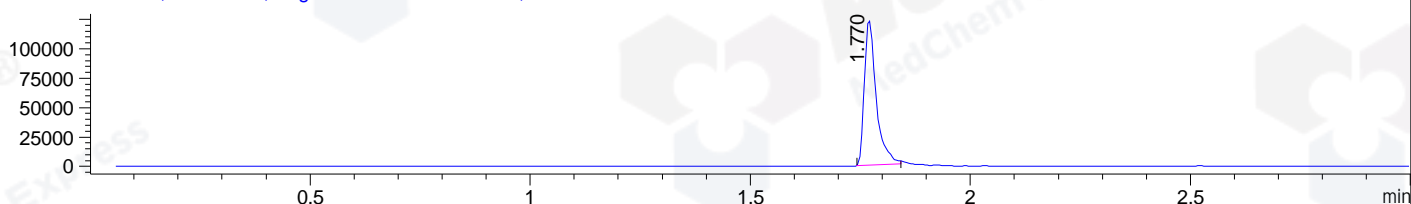

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.51	0.02	12.34	12.07	0.78	339
1.76	0.02	1555.08	1359.47	98.88	491
1.96	0.02	5.26	5.49	0.33	159

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.51	0.02	7.68	7.70	1.26	339
1.76	0.02	597.93	548.64	98.33	491
1.96	0.02	2.47	2.53	0.41	159

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.77	0.03	779629.13	383013.31	100.00	491

Ret. Time: 1.77

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

