



File ..\DATA\2020\20200507\948\CPK2020-506-07195.D Tgt Mass (CHM):  
Injection Date : 7 May 20 2:09 pm +0800 Seq. Line : 37  
Sample Name : CPK2020-506-07195 Location : P1-F-02  
Acq. Operator : ZJ\_1432 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2020\20200507\948\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2020\20200507\948\1-POS-3MIN.M  
Catalog No : HY-17368  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

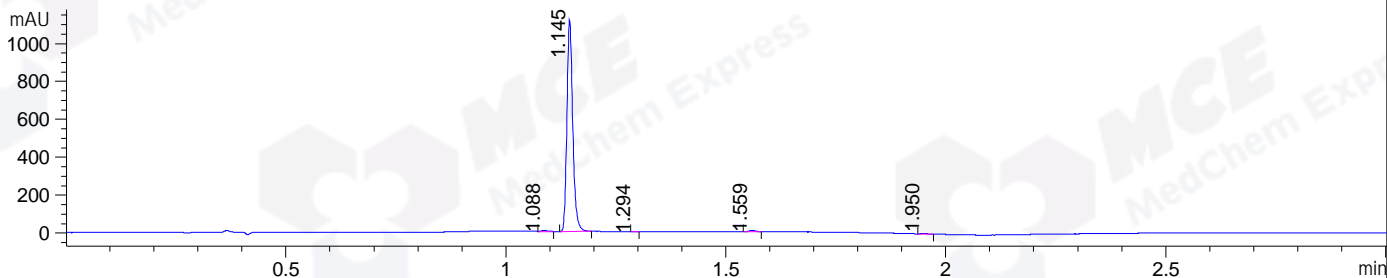

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

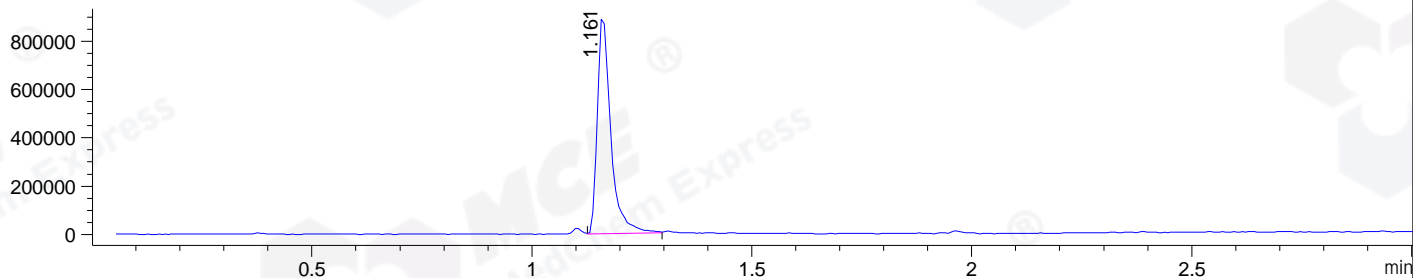

Ion 251, MSD1 251, Target Mass 250 +H Positive, EIC=250.7:251.7

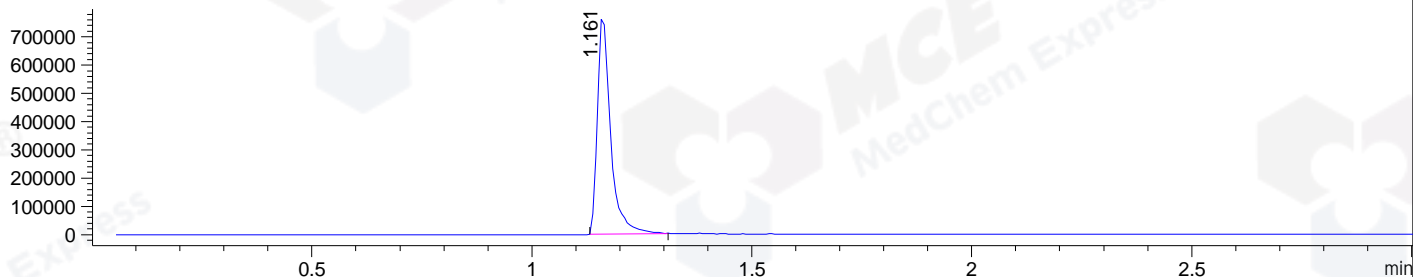

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.09	0.01	4.05	5.16	0.39	237
1.14	0.02	1025.55	1117.53	98.75	251
1.29	0.01	0.41	0.79	0.04	251
1.56	0.01	5.54	6.21	0.53	251
1.95	0.02	2.98	3.04	0.29	242

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.16	0.03	1933467.50	908657.31	100.00	251

Ret. Time: 1.16

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

