



File ..DATA\2020\20201215\1201\CPK2020-D15-07892.D Tgt Mass (CHM):
Injection Date : 15 Dec 20 9:41 pm +0800 Seq. Line : 132
Sample Name : CPK2020-D15-07892 Location : P1-C-05
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20201215\1201\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20201215\1201\1-POS-3MIN.M
CAS NO. : 1977-10-2
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

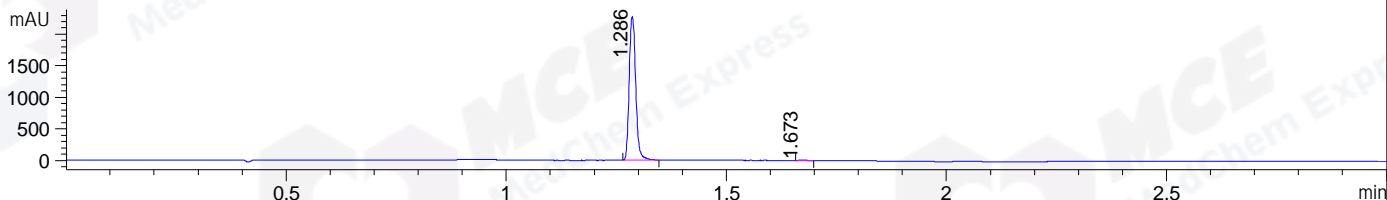


DAD1 C, Sig=254,4 Ref=off

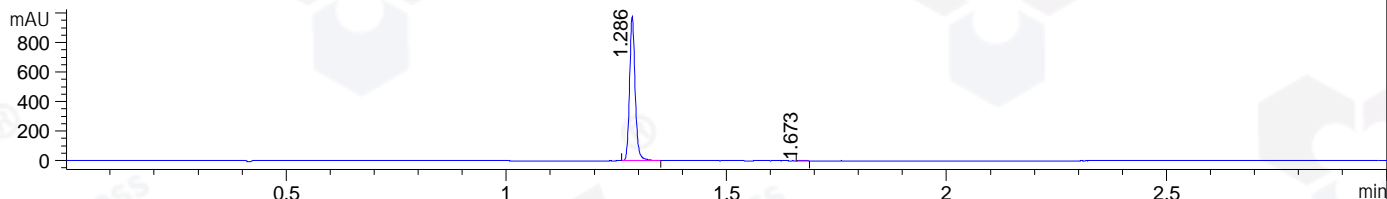

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

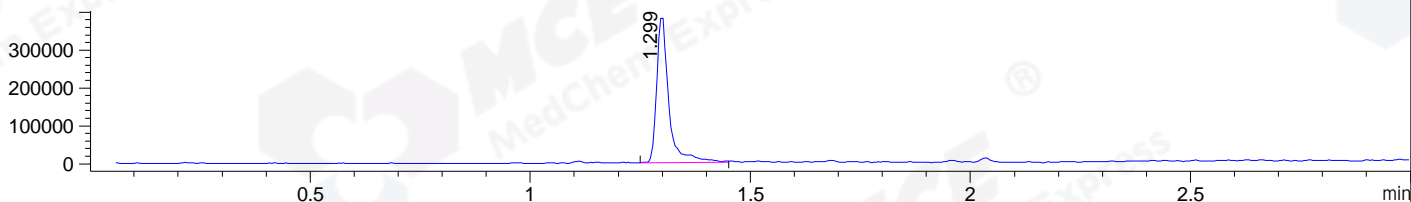

Ion 328, MSD1 328, Target Mass 327 +H Positive, EIC=327.7:328.7

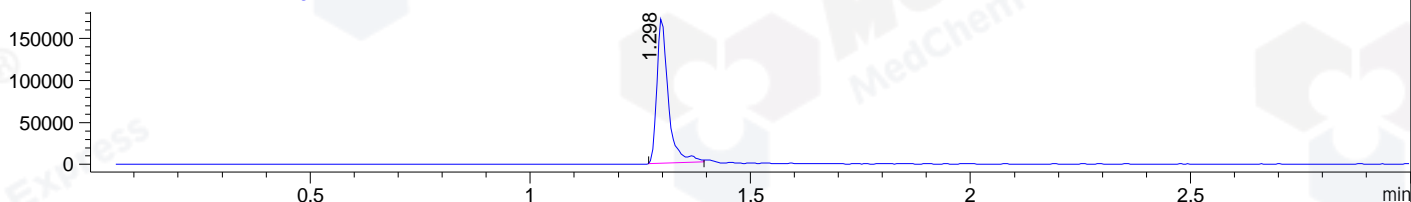

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.29	0.02	2348.78	2278.37	99.49	328
1.67	0.02	11.96	12.29	0.51	308

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.29	0.01	865.30	980.14	99.88	328
1.67	0.02	1.06	1.15	0.12	308

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.30	0.03	741569.69	390481.13	100.00	328

Ret. Time: 1.30

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

