



File ..ATA\2020\20200903\1097\CPK2020-902-61625-.D Tgt Mass (CHM):
Injection Date : 3 Sep 20 9:25 pm +0800 Seq. Line : 150
Sample Name : CPK2020-902-61625 Location : P1-B-04
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.5 ul
Acq. Method : D:\Chem32\1\data\2020\20200903\1097\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20200903\1097\1-POS-3MIN.M
Catalog No : HY-18062
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

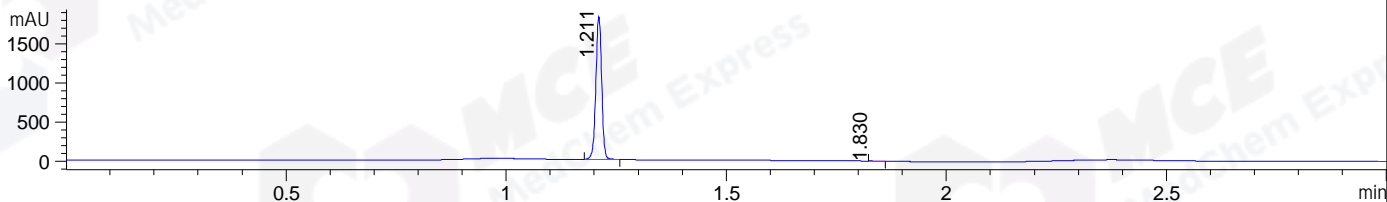


DAD1 C, Sig=254,4 Ref=off

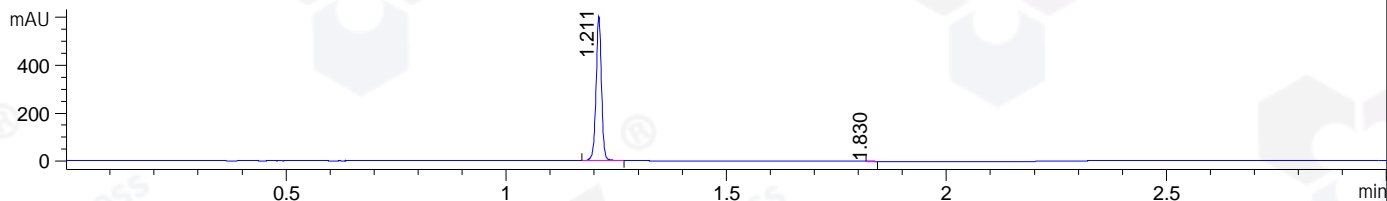

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

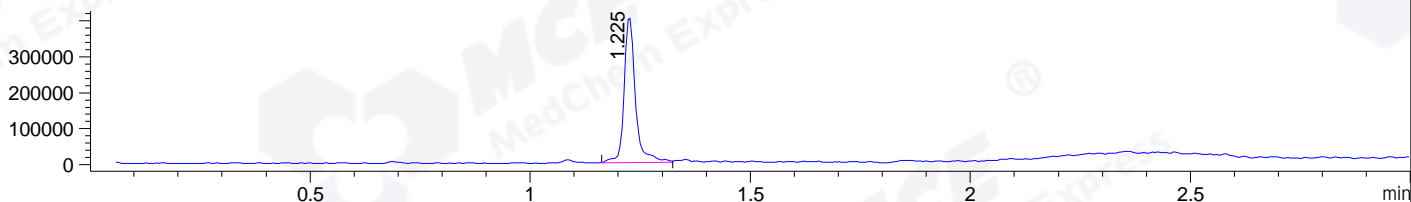

Ion 249, MSD1 249, Target Mass 248 +H Positive, EIC=248.7:249.7

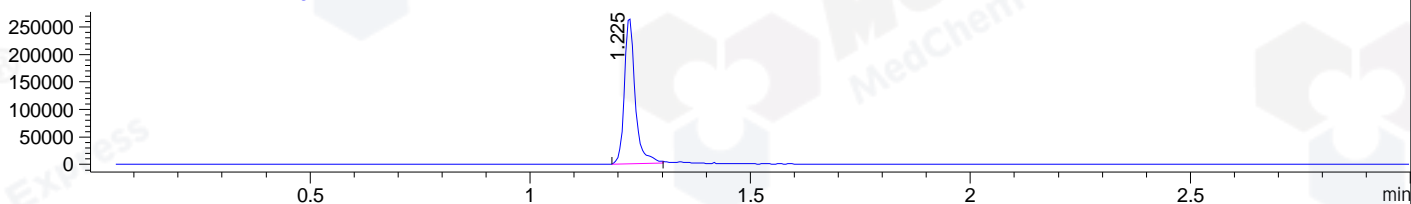

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.21	0.02	1698.55	1827.58	99.86	249
1.83	0.03	2.46	1.57	0.14	297

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.21	0.01	516.17	602.84	99.94	249
1.83	0.02	0.31	0.33	0.06	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.23	0.03	728399.81	409724.41	100.00	249

Ret. Time: 1.23

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

