



File ..\DATA\2019\20190823\705\CPK2019-822-11459.D Tgt Mass (CHM):
 Injection Date : 24 Aug 19 9:16 am +0800 Seq. Line : 4
 Sample Name : CPK2019-822-11459 Location : P1-B-07
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2019\20190823\705\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2019\20190823\705\1-POS-3MIN.M
 Catalog No : HY-18306 Batch#11459
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

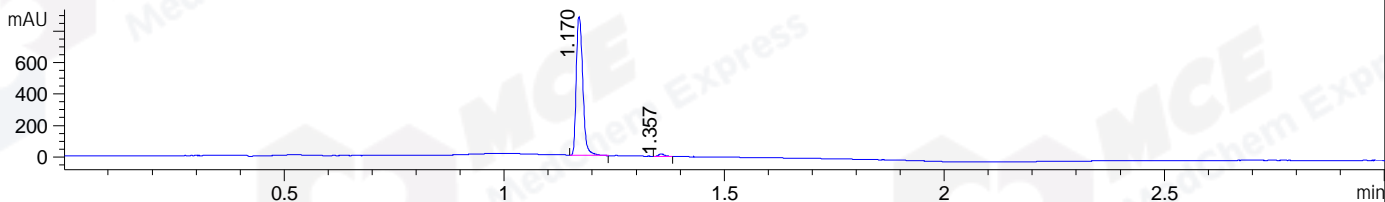


DAD1 C, Sig=254,4 Ref=off

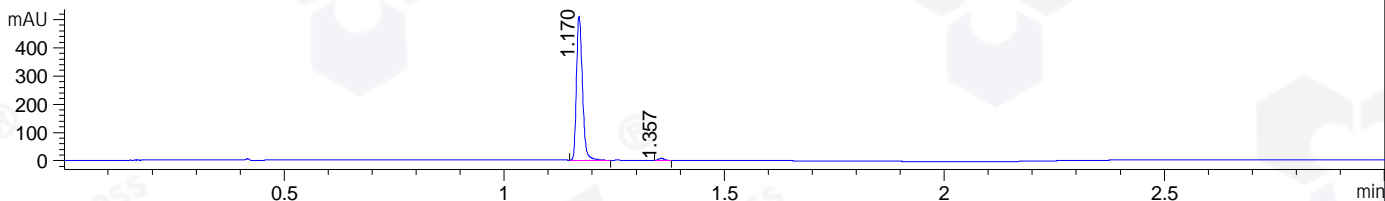

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

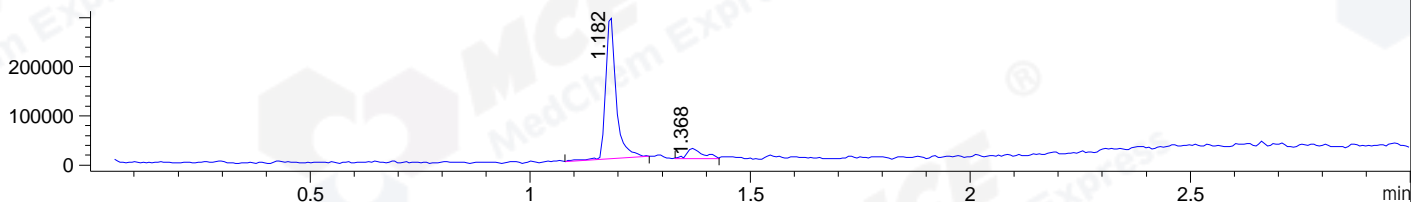

Ion 354.4026, MSD1 354.4026, Target Mass 353.4026 +H Positive, EIC=354.10:355.10

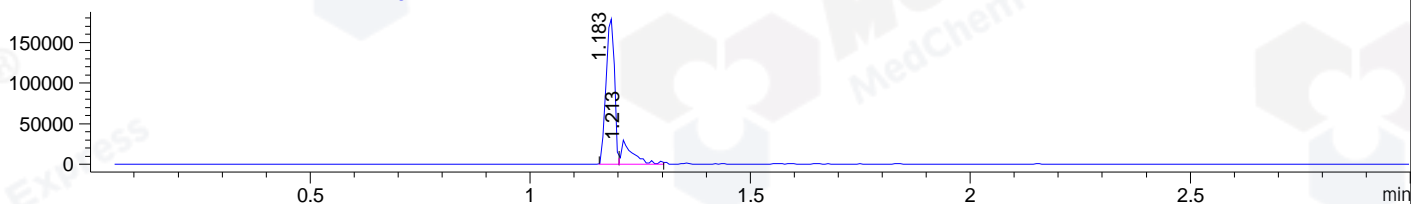

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.02	907.05	882.98	98.50	354
1.36	0.01	13.85	15.48	1.50	393

Integration Results for DAD1 C, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.02	479.50	510.81	98.63	354
1.36	0.01	6.66	7.46	1.37	393

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.18	0.02	481622.28	296311.59	90.01	354
1.37	0.04	53450.22	20829.84	9.99	393

Ret. Time: 1.18

<<<< POSITIVE SPECTRA >>>>

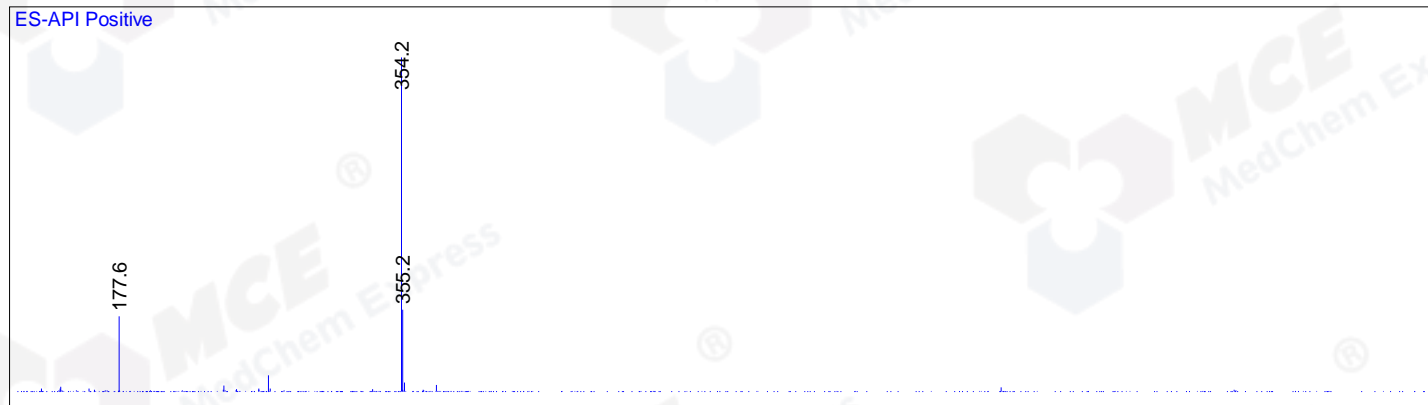

Ret. Time: 1.37

