



File ..DATA\2020\20200813\1068\BIZ2020-810-WLQ3-.D Tgt Mass (CHM):
 Injection Date : 13 Aug 20 9:21 am +0800 Seq. Line : 5
 Sample Name : BIZ2020-810-WLQ3 Location : P1-D-04
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.3 ul
 Acq. Method : D:\Chem32\1\data\2020\20200813\1068\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200813\1068\1-POS-3MIN.M
 Catalog No : HY-18341B
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

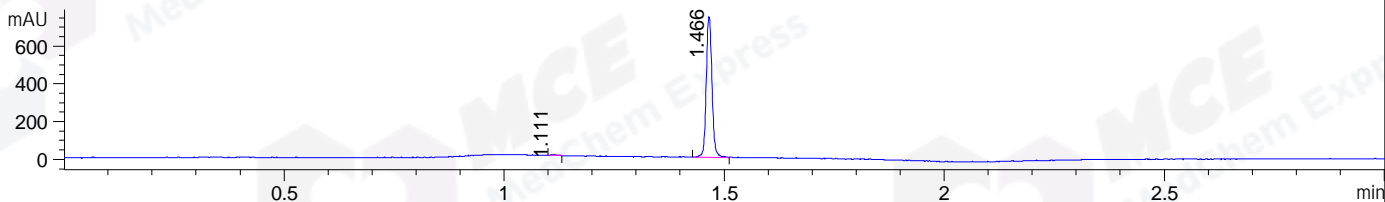


DAD1 C, Sig=254,4 Ref=off

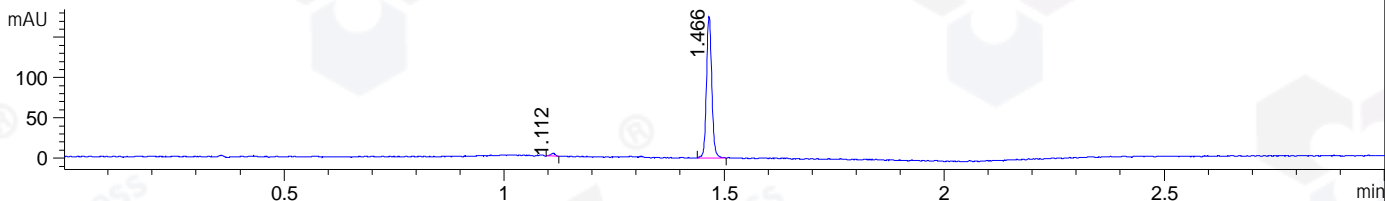

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

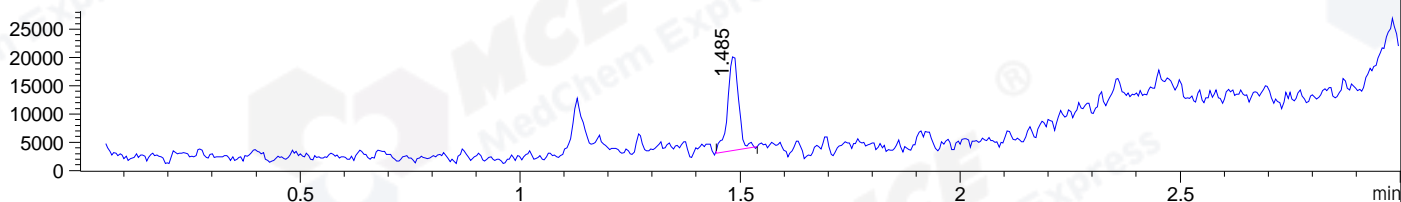

Ion 777, MSD1 777, Target Mass 776 +H Positive, EIC=776.7:777.7

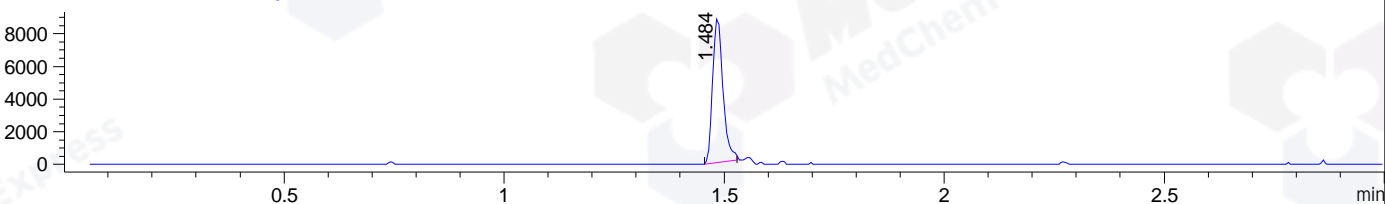

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.11	0.01	3.89	5.28	0.57	210
1.47	0.02	674.38	746.66	99.43	778

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.11	0.01	2.11	3.20	1.42	210
1.47	0.01	146.74	176.25	98.58	778

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.48	0.02	28618.22	16638.07	100.00	778

Ret. Time: 1.48

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

