


=====
Acq. Operator : Yang Qian(LCMS-02) Seq. Line : 29
Acq. Instrument : HY-LCMS-02 Location : P1-C-09
Injection Date : 10/19/2015 2:05:27 PM Inj : 1
Inj Volume : 3.000 µl
Acq. Method : D:\AGLIENT 1260\DATA\20151019\20151019 2015-10-19 09-14-11\100-1000MS+3MIN-1.5_(0.02%FA).M
Last changed : 10/19/2015 9:14:11 AM by Yang Qian(LCMS-02)
Analysis Method : D:\AGLIENT 1260\DATA\20151012\20151012 2015-10-12 13-29-27\100-1000MS+3MIN-1.5_(0.02%FA).M (Sequence Method)
Last changed : 10/19/2015 2:35:04 PM by Yang Qian(LCMS-02)
(modified after loading)
Method Info : Postive,MS:100-1000,Column ID:A-RP-132,40°C
Catalog No : HY-18690 Batch#18195
A-RP-134

Additional Info : Peak(s) manually integrated

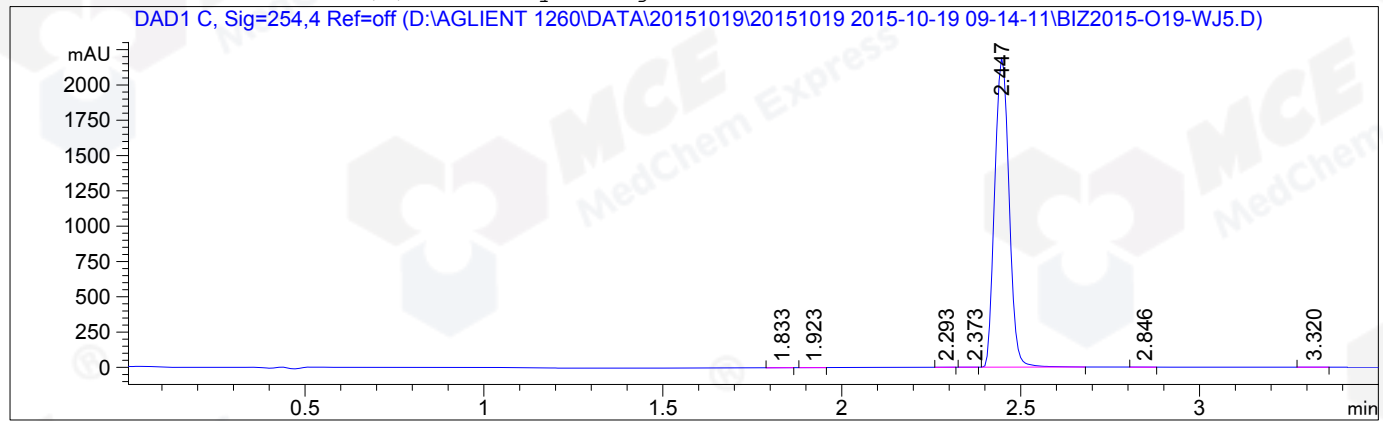

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 C, Sig=254,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.833	MM	0.0522	5.31643e-1	1.69634e-1	8.704e-3
2	1.923	MM	0.0418	2.14133	8.53855e-1	0.0351
3	2.293	MM	0.0453	4.63596e-1	1.70640e-1	7.590e-3
4	2.373	MM	0.0367	6.54560e-1	2.97368e-1	0.0107
5	2.447	MM	0.0462	6102.38867	2203.29834	99.9055
6	2.846	MM	0.0481	8.63917e-1	2.99227e-1	0.0141
7	3.320	MM	0.0605	1.11675	3.07541e-1	0.0183


Totals : 6108.16047 2205.39661

=====
*** End of Report ***

=====


Acq. Operator	: Yang Qian (LCMS-02)	Seq. Line	: 29
Acq. Instrument	: HY-LCMS-02	Location	: P1-C-09
Injection Date	: 10/19/2015 2:05:27 PM	Inj	: 1
		Inj Volume	: 3.000 µl
Acq. Method	: D:\AGLIENT 1260\DATA\20151019\20151019 2015-10-19 09-14-11\100-1000MS+3MIN-1.5_(0.02%FA).M		
Last changed	: 10/19/2015 9:14:11 AM by Yang Qian (LCMS-02)		
Analysis Method	: D:\AGLIENT 1260\DATA\20151012\20151012 2015-10-12 13-29-27\100-1000MS+3MIN-1.5_(0.02%FA).M (Sequence Method)		
Last changed	: 10/19/2015 2:44:19 PM by Yang Qian (LCMS-02) (modified after loading)		
Method Info	: Postive,MS:100-1000,Column ID:A-RP-132,40°C		
Catalog No	: HY-18690 Batch#18195 A-RP-134		

Additional Info : Peak(s) manually integrated

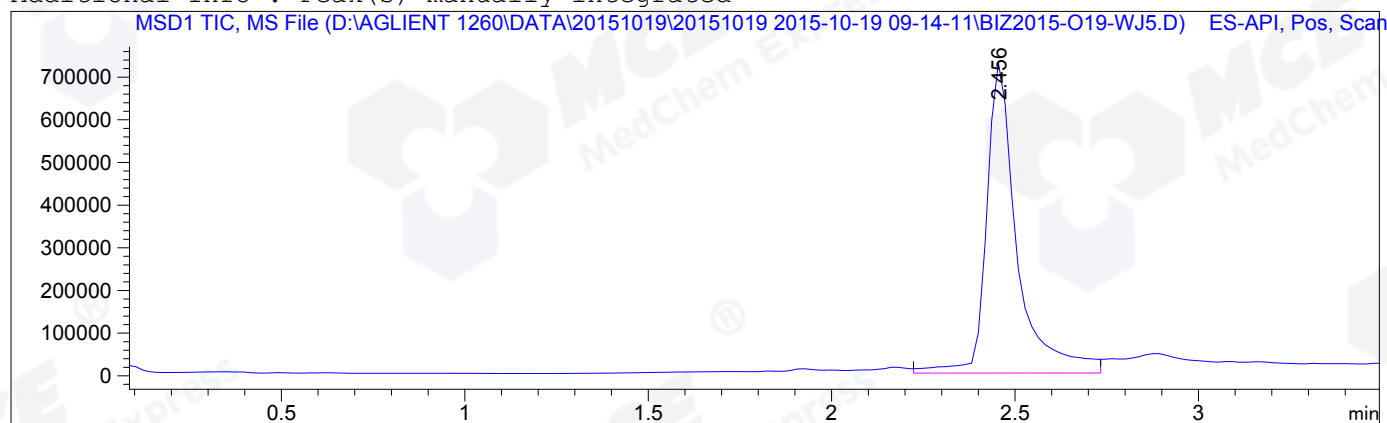

MS Signal: MSD1 TIC, MS File, ES-API, Pos, Scan, Frag: 50
Spectra averaged over upper half of peaks.
Noise Cutoff: 1000 counts.
Reportable Ion Abundance: > 10%.

Retention Time (MS)	MS Area	Mol. Weight or Ion
2.456	4234898	475.20 I
		474.20 I

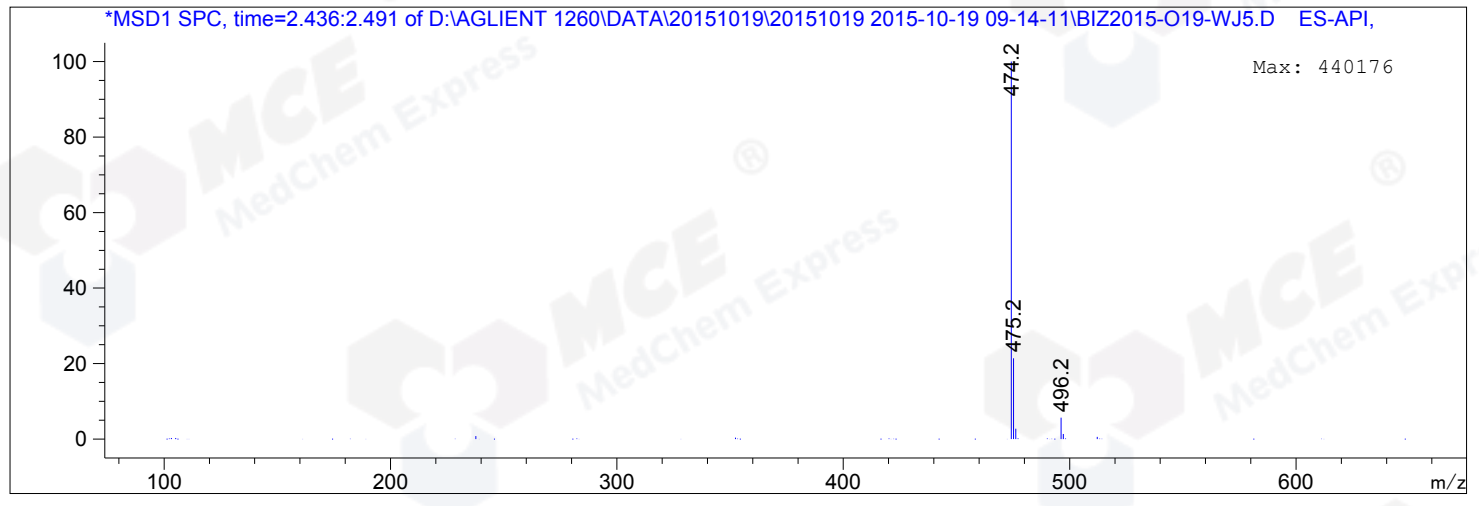

*** End of Report ***