



File ..\DATA\2019\20190809\682\CPK2019-808-22449.D Tgt Mass (CHM):  
 Injection Date : 9 Aug 19 10:59 am +0800 Seq. Line : 24  
 Sample Name : CPK2019-808-22449 Location : P1-A-05  
 Acq. Operator : ZJ\_1432 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2019\20190809\682\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2019\20190809\682\1-POS-3MIN.M  
 Catalog No : HY-18780 Batch#22449  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433  
 Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

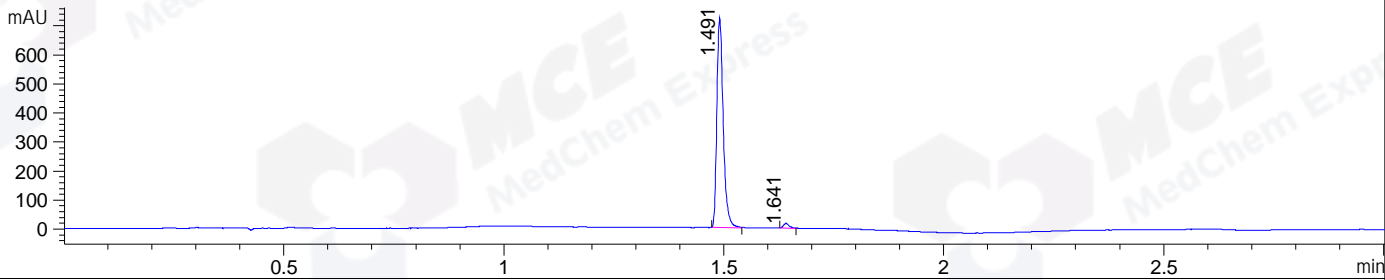

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

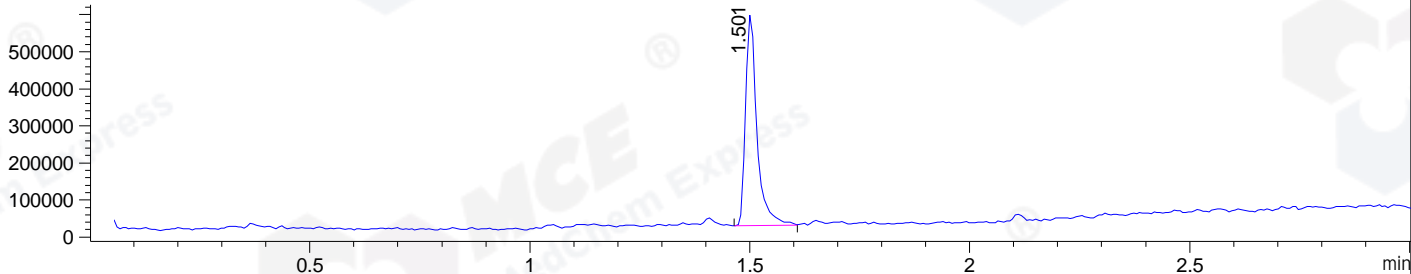

Ion 294.366, MSD1 294.366, Target Mass 293.366 +H Positive, EIC=294.07:295.07

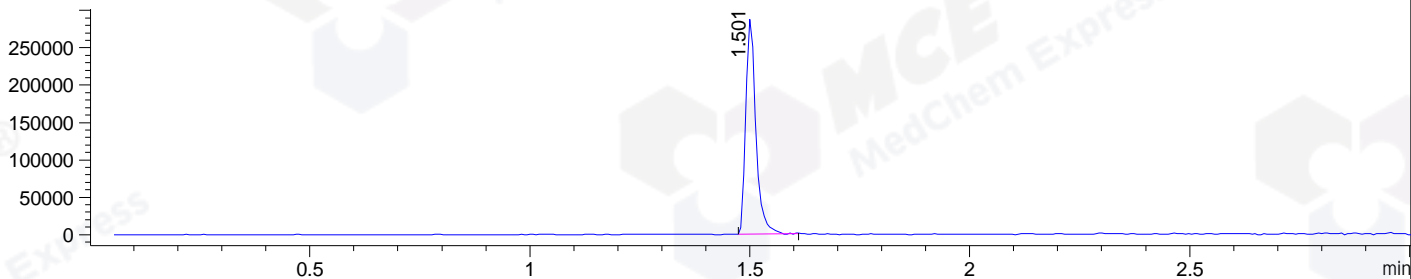

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.49	0.02	727.96	722.06	97.95	294
1.64	0.01	15.23	16.62	2.05	130

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.50	0.03	1030596.25	572049.50	100.00	294

Ret. Time: 1.50

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

